



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Capaldi Ranch/Daphne Capaldi
872 Exline Rd
Paso Robles CA 93446 USA

Date: 06/03/13

Test No: 454836


Animal and Sample Description

Animal Name: Lincoln
Breed: Alpaca(Huacaya)
Sex: Female
Color: Grey

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/13/13
Age: 10/2011

Laboratory Data

Mean Fiber Diameter:	19.8 microns	Fibers Greater Than 30 microns:	2.6 %
Standard Deviation:	4.5 microns	Comfort Factor:	97.4 %
Coefficient of Variation:	22.5 %	Mean Curvature:	41.0 deg/mm
Spin Fineness:	19.6 microns	SD Curvature:	25.0 deg/mm

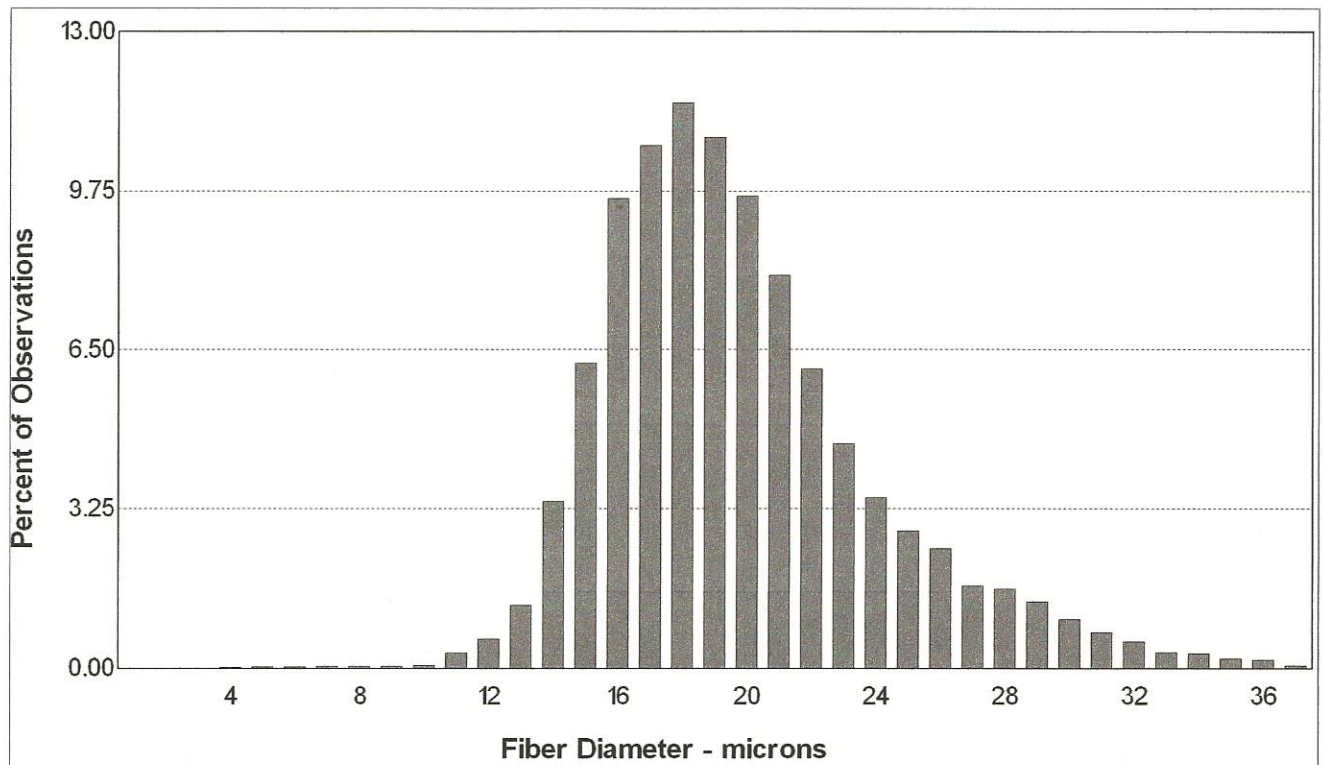

This Test Performed According to I.W.T.O Method 47