



Yocom-McColl Testing Laboratories, Inc.  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)  
Micron Test Report**

Volcano Accoyos/Jim Edwards  
81 Franklin Court  
La Porte IN 46350 USA

09/12/13

**Test No:** 469389


**Animal and Sample Description**

**Animal Name:** Shangri-La's Felice  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Silver Grey

**Animal ID:** 32768503  
**Sample Location:** Side (R)  
**Sample Date:** 05/24/13  
**Age:** 07/28/12

**Laboratory Data**

<b>Mean Fiber Diameter:</b>	17.4 microns	<b>Spin Fineness:</b>	16.5 microns
<b>Standard Deviation:</b>	3.1 microns	<b>Mean Curvature (deg/mm):</b>	35.6
<b>Coefficient of Variation:</b>	18.0 %	<b>SD Curvature (deg/mm):</b>	23.0
<b>Fibers Greater Than 30 microns:</b>	0.3 %	<b>Comfort Factor:</b>	99.7 %

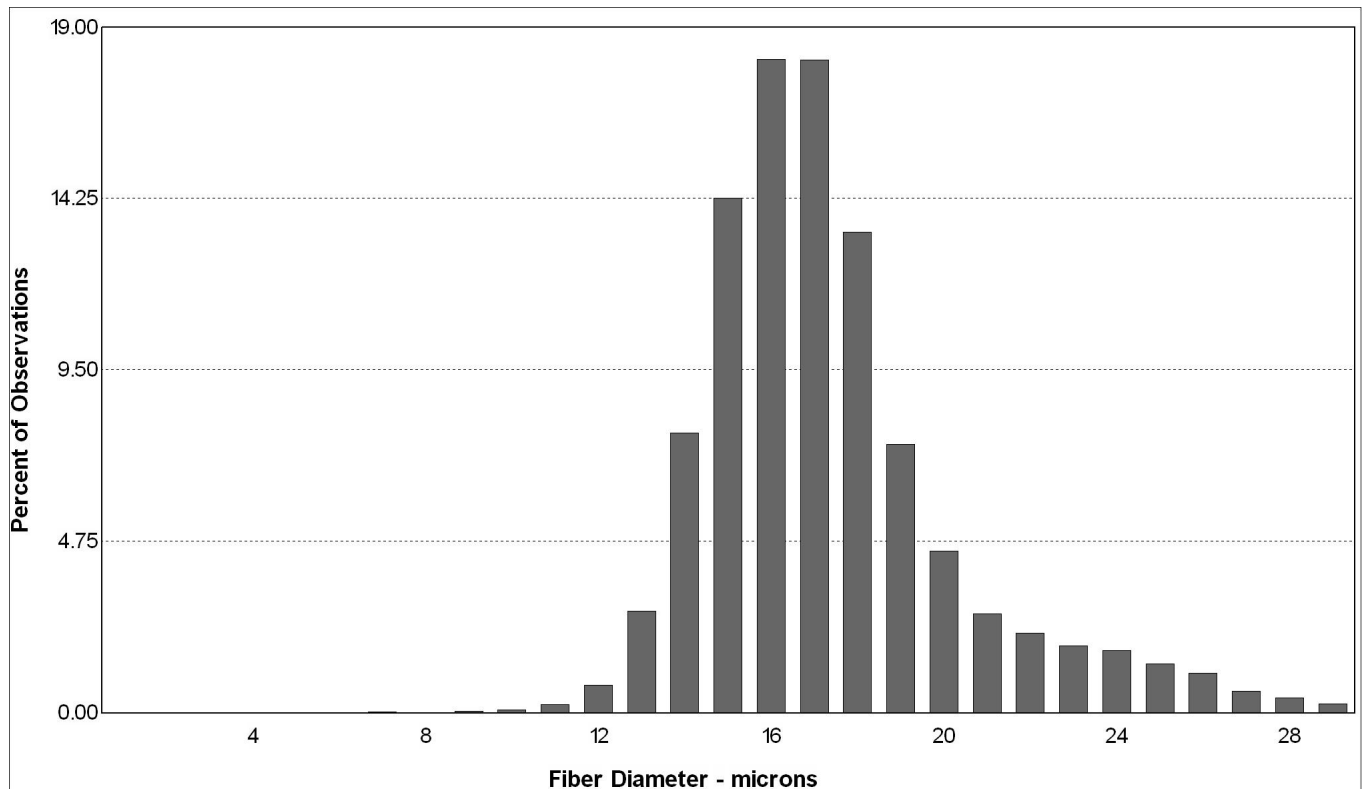

**This Test Performed According to I.W.T.O Method 47**