



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan  
Micron Test Report

Skyline Alpacas/Mary Jaffe  
11100 NW Saltzman Rd  
Portland OR 97229 USA

07/08/16

Test No: 926390


## Animal and Sample Description

**Animal Name:** Gentian  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Silver Grey

**Animal ID:** 30635319  
**Sample Location:** Side  
**Sample Date:** 05/04/16  
**Age:** 10/14/09

## Laboratory Data

**Mean Fiber Diameter:** 22.4 microns  
**Standard Deviation:** 5.5 microns  
**Coefficient of Variation:** 24.5 %  
**Fibers Greater Than 30 microns:** 8.3 %

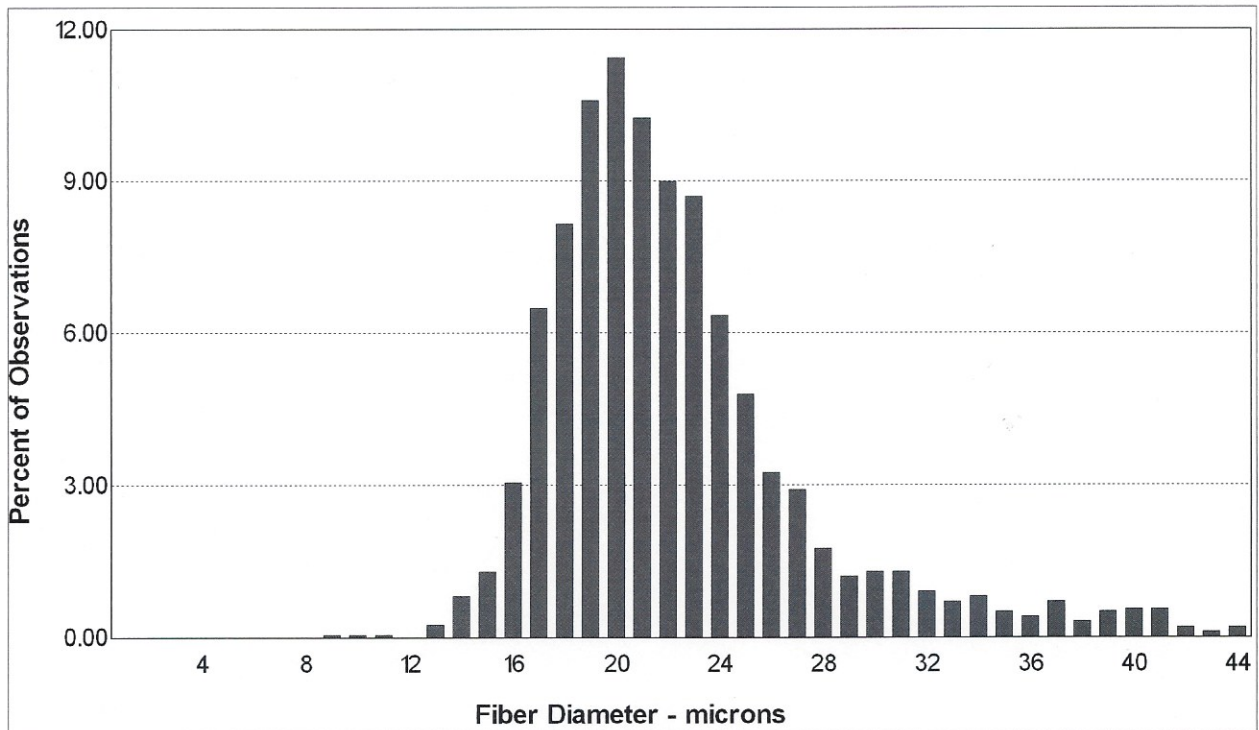

This Test Performed According to I.W.T.O Method 12