



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Skyline Alpacas/Mary Jaffe
11100 NW Saltzman Rd
Portland OR 97229 USA

08/05/13

Test No: 464106


Animal and Sample Description

Animal Name: Red Swan
Breed: Alpaca(Huacaya)
Sex: Female
Color: Dark Brown

Animal ID: 32735031
Sample Location: Side
Sample Date: 05/02/13
Age: 06/14/12

Laboratory Data

Mean Fiber Diameter: 20.0 microns
Standard Deviation: 4.6 microns
Coefficient of Variation: 22.9 %
Fibers Greater Than 30 microns: 3.1 %

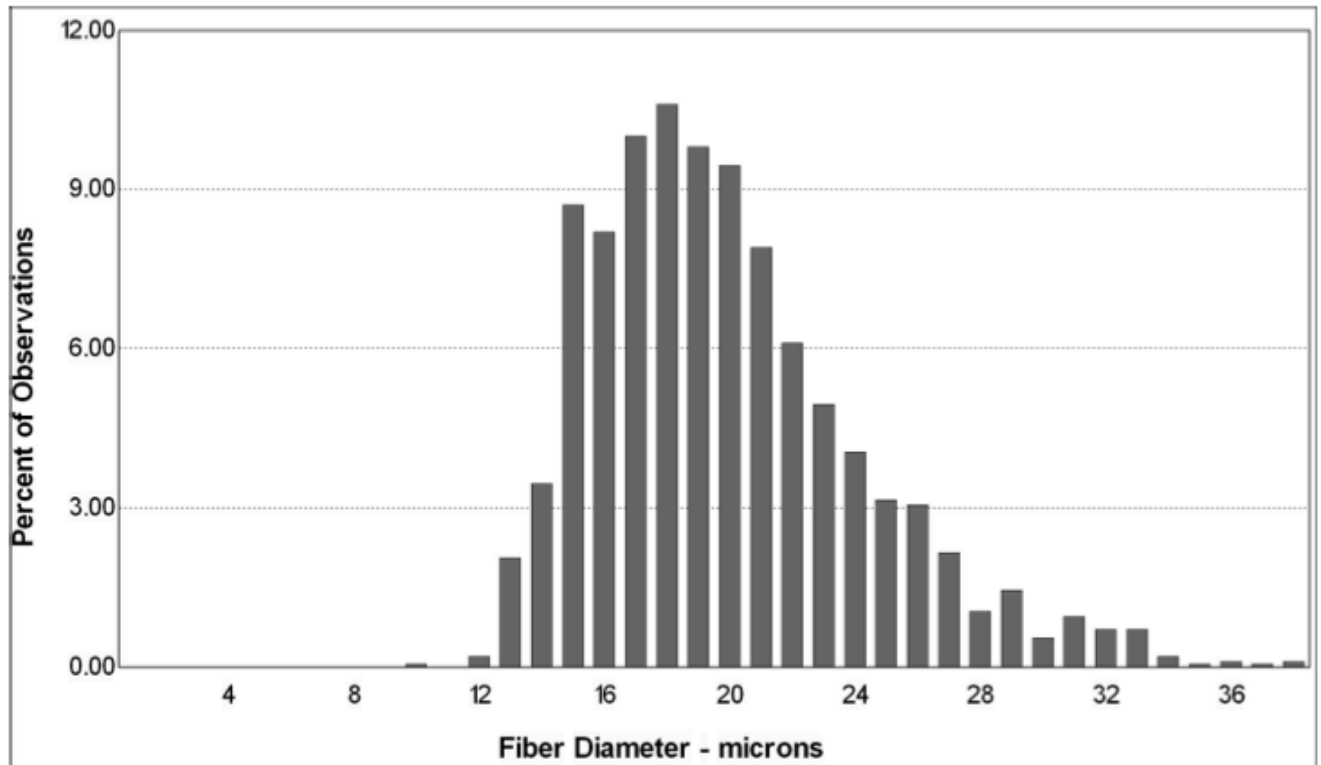

This Test Performed According to I.W.T.O Method 12