



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Skyline Alpacas/Mary Jaffe  
11100 NW Saltzman Rd  
Portland OR 97229 USA

06/21/17

Test No: 943685


### Animal and Sample Description

**Animal Name:** Yukon  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Silver Grey

**Animal ID:** 35314486  
**Sample Location:** Side  
**Sample Date:** 05/16/17  
**Age:** 07/04/16

### Laboratory Data

**Mean Fiber Diameter:** 17.4 microns  
**Standard Deviation:** 3.0 microns  
**Coefficient of Variation:** 17.5 %  
**Fibers Greater Than 30 microns:** 0.8 %

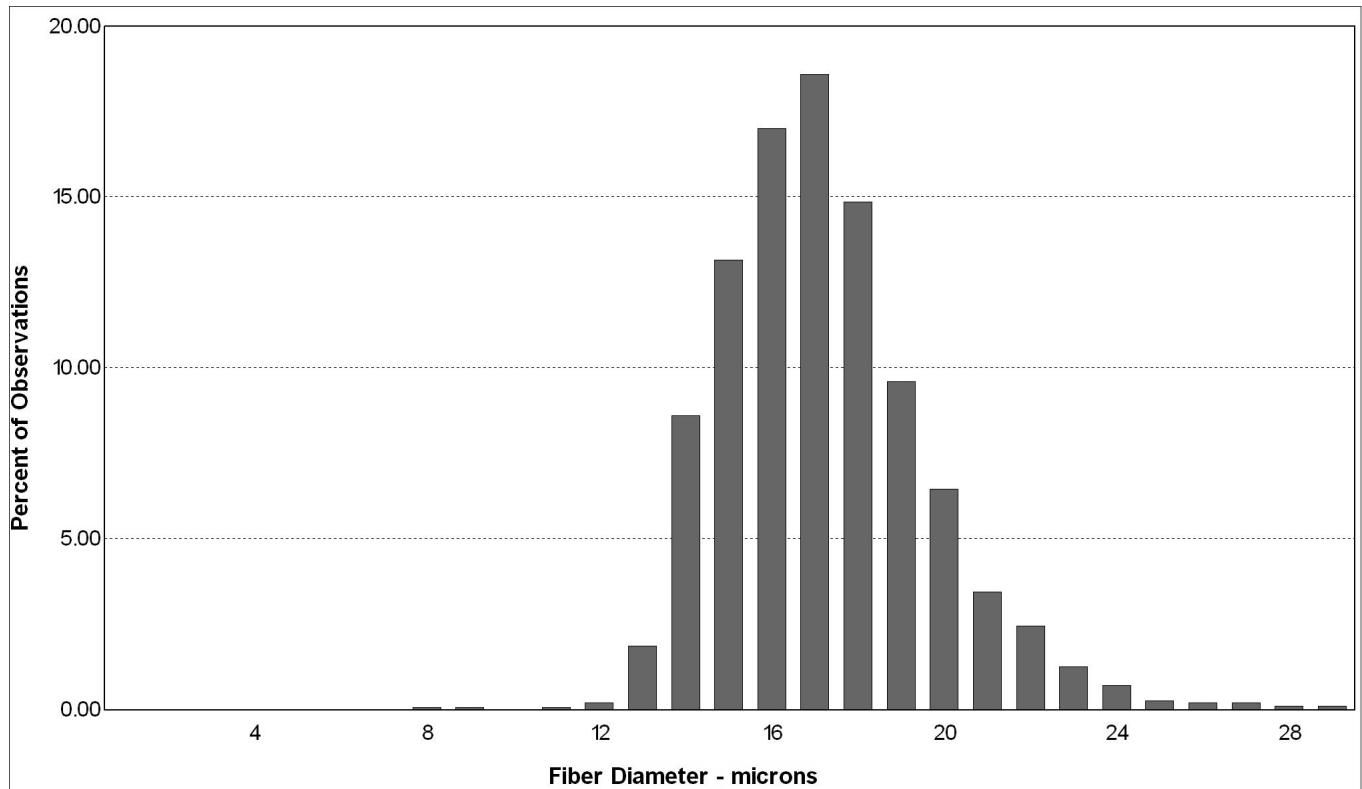

This Test Performed According to I.W.T.O Method 12