



**Yocom-McColl Testing Laboratories, Inc.**  
 540 West Elk Place • Denver, Colorado 80216-1823 USA  
 PHONE (303) 294-0582 • FAX (303) 295-6944  
 EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan  
 Micron Test Report**

Sugarland Ranch/Aaron & Connie Konrardy  
 18539 Hwy 52 North  
 Durango IA 52039 USA

09/05/19

Test No: 983236


**Animal and Sample Description**

**Animal Name:** Sugarland's Highlandar  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 35490371  
**Sample Location:** Side  
**Sample Date:** 04/29/19  
**Age:** 06/09/18

**Laboratory Data**

**Mean Fiber Diameter:** 17.5 microns  
**Standard Deviation:** 3.9 microns  
**Coefficient of Variation:** 22.0 %  
**Fibers Greater Than 30 microns:** 0.8 %

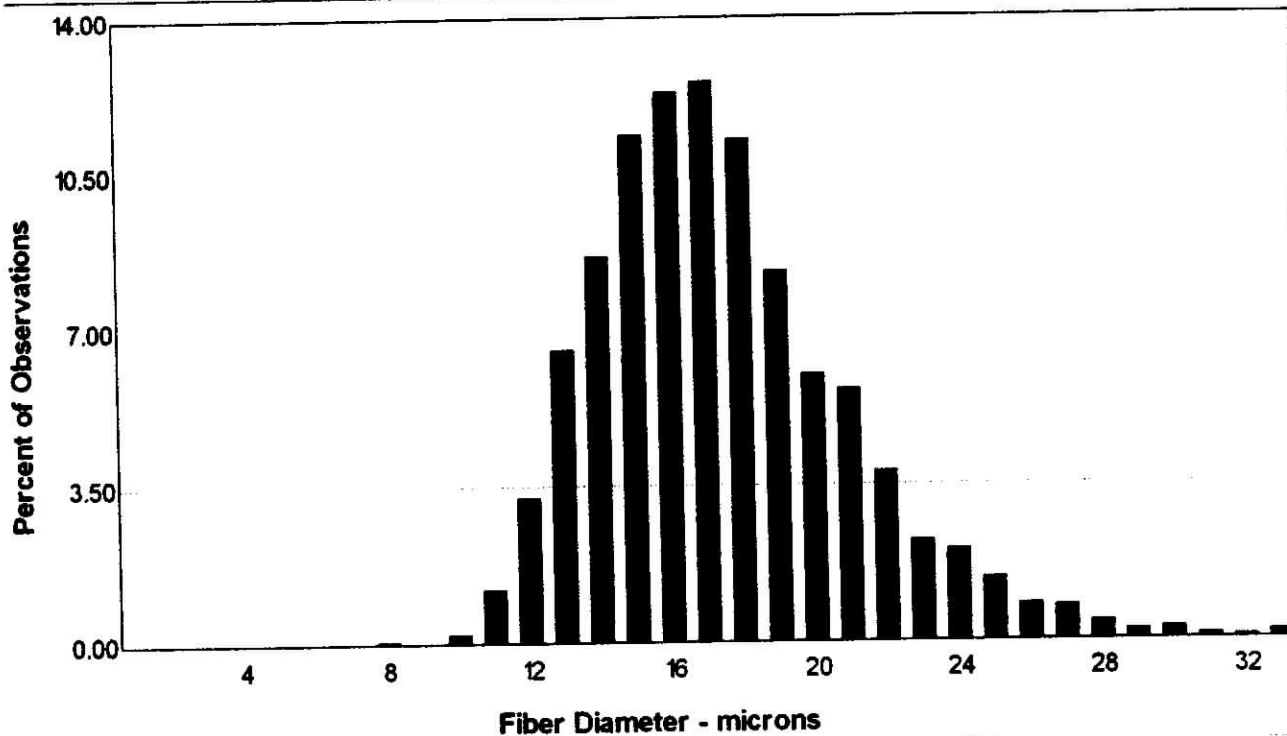

**This Test Performed According to I.W.T.O Method 12**