



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault  
411 Brill Road, RR32  
West Bolton QC J0E 2T0 Canada

12/28/17

Test No: 955963


### Animal and Sample Description

**Animal Name:** Maringo Cloud-CA109's Cria (2017)  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Rose Grey

**Animal ID:** XXXXX  
**Sample Location:** Side  
**Sample Date:** 12/17/17  
**Age:** 08/11/17

### Laboratory Data

<b>Mean Fiber Diameter:</b>	17.6 microns	<b>Spin Fineness:</b>	16.9 microns
<b>Standard Deviation:</b>	3.4 microns	<b>Mean Curvature (deg/mm):</b>	36.8
<b>Coefficient of Variation:</b>	19.6 %	<b>SD Curvature (deg/mm):</b>	28.8
<b>Fibers Greater Than 30 microns:</b>	0.5 %	<b>Comfort Factor:</b>	99.5 %

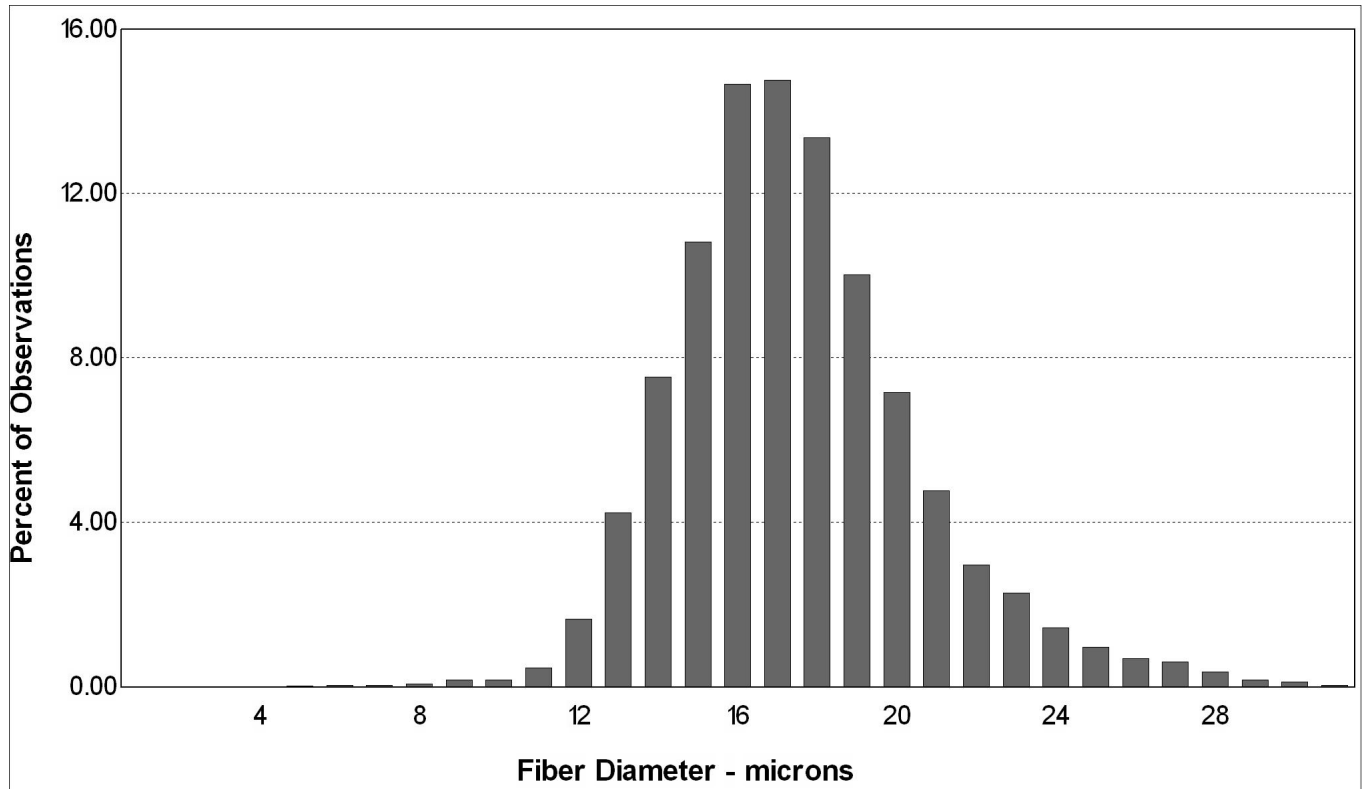

This Test Performed According to I.W.T.O Method 47