



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Brill Road, RR32
West Bolton QC J0E 2T0 Canada

Date: 04/11/17

Test No: 940594


Animal and Sample Description

Animal Name: J.A. Pure Reserve's Arthgallo
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Fawn

Animal ID: 30722590
Sample Location: Side
Sample Date: 04/02/17
Age: 06/11/16

Laboratory Data

Mean Fiber Diameter:	15.6 microns	Fibers Greater Than 30 microns:	0.3 %
Standard Deviation:	3.8 microns	Comfort Factor:	99.7 %
Coefficient of Variation:	24.0 %	Mean Curvature:	42.5 deg/mm
Spin Fineness:	15.6 microns	SD Curvature:	30.4 deg/mm

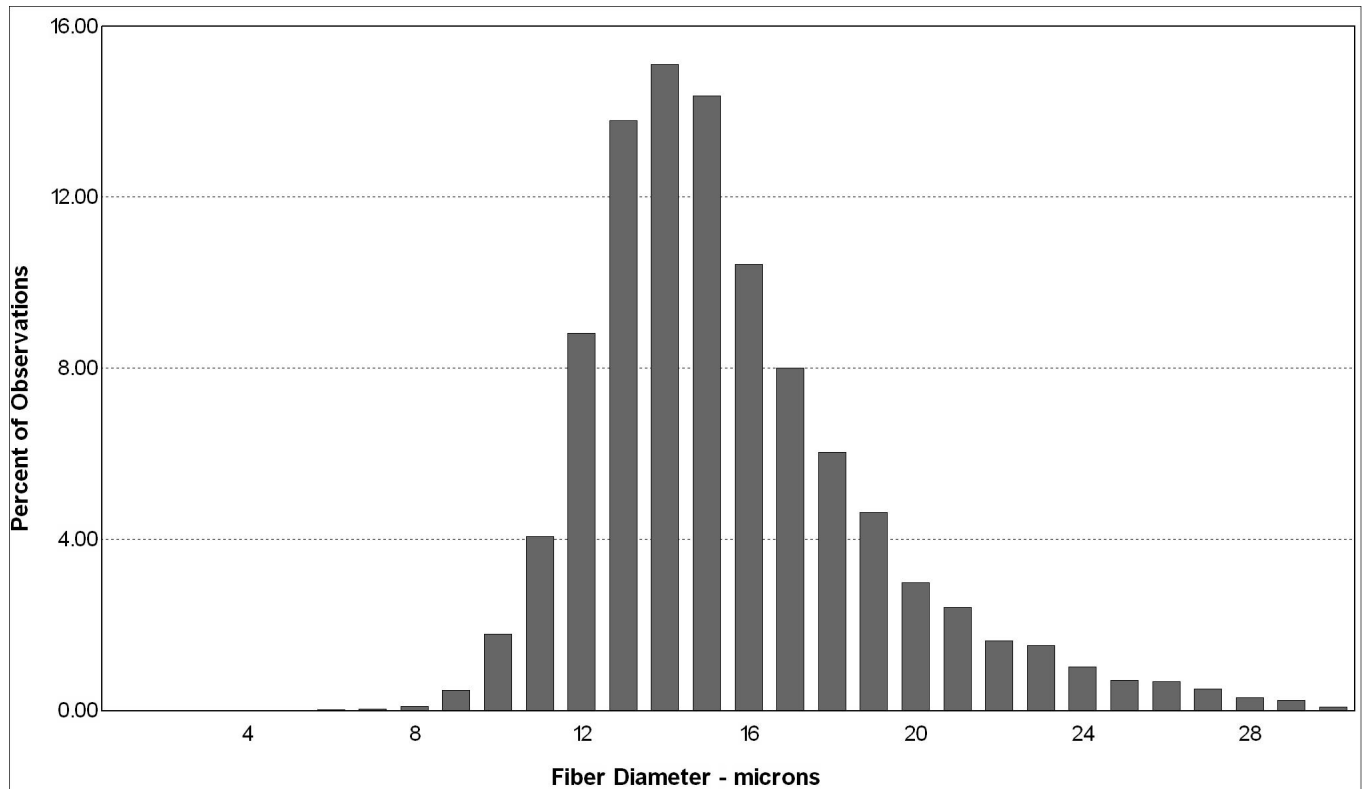

This Test Performed According to I.W.T.O Method 47