



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Chemin De Brill Road, RR32
Bolton Ouest QC J0E 2T0 Canada

Date: 08/05/18

Test No: 965431


Animal and Sample Description

Animal Name: Chicha
Breed: Alpaca(Huacaya)
Sex: Female
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/28/18
Age: XXXXX

Laboratory Data

Mean Fiber Diameter:	19.2 microns	Fibers Greater Than 30 microns:	0.4 %
Standard Deviation:	3.1 microns	Comfort Factor:	99.6 %
Coefficient of Variation:	16.2 %	Mean Curvature:	44.6 deg/mm
Spin Fineness:	18.0 microns	SD Curvature:	24.5 deg/mm

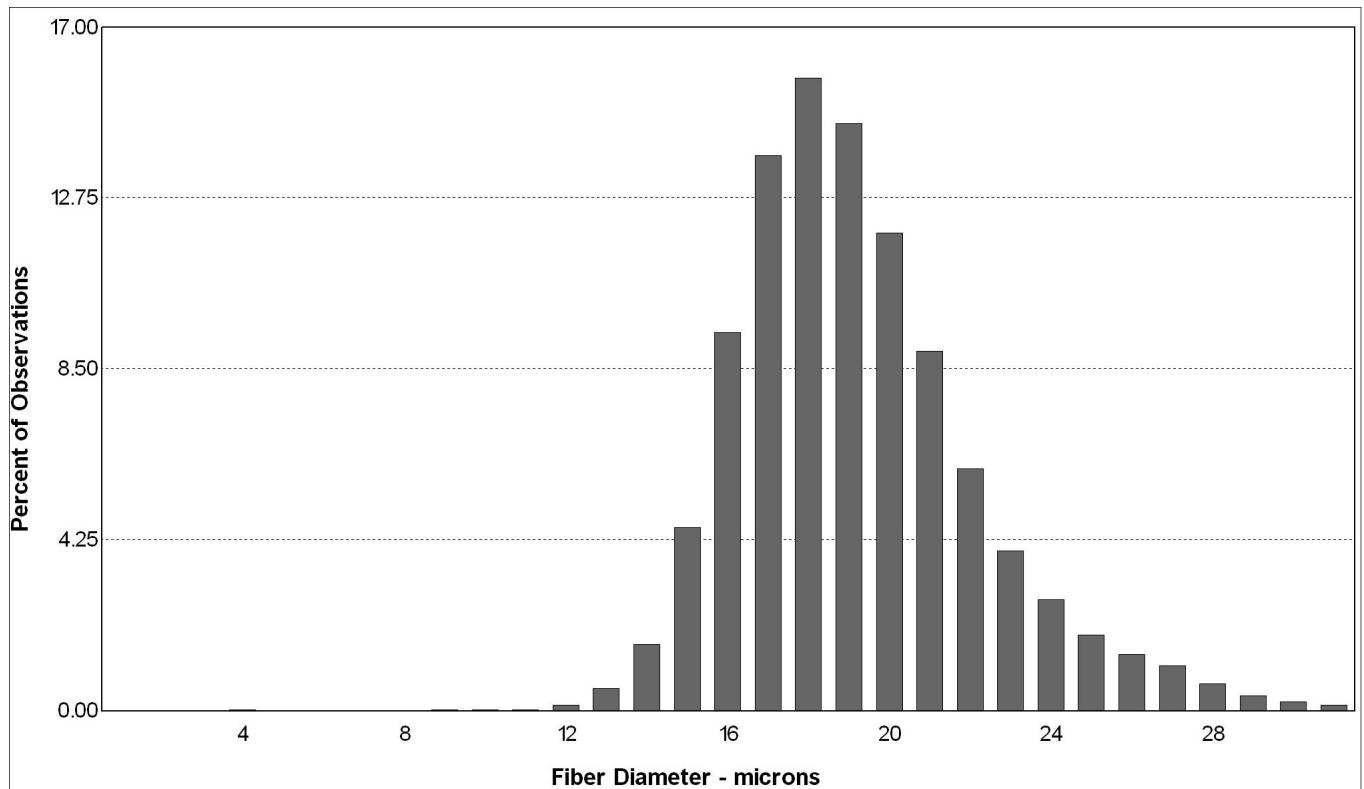

This Test Performed According to I.W.T.O Method 47