



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault  
411 Brill Road  
West Bolton QC J0E 2T0 Canada

**Date:** 07/12/19

**Test No:** 976924


### Animal and Sample Description

**Animal Name:** Ariya Domain's Simple Pleasure  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Beige

**Animal ID:** XXXXX  
**Sample Location:** Mid Side  
**Sample Date:** 05/05/19  
**Age:** 07/14/18

### Laboratory Data

<b>Mean Fiber Diameter:</b>	16.4 microns	<b>Fibers Greater Than 30 microns:</b>	1.0 %
<b>Standard Deviation:</b>	3.8 microns	<b>Comfort Factor:</b>	99.0 %
<b>Coefficient of Variation:</b>	22.9 %	<b>Mean Curvature:</b>	52.2 deg/mm
<b>Spin Fineness:</b>	16.2 microns	<b>SD Curvature:</b>	28.6 deg/mm

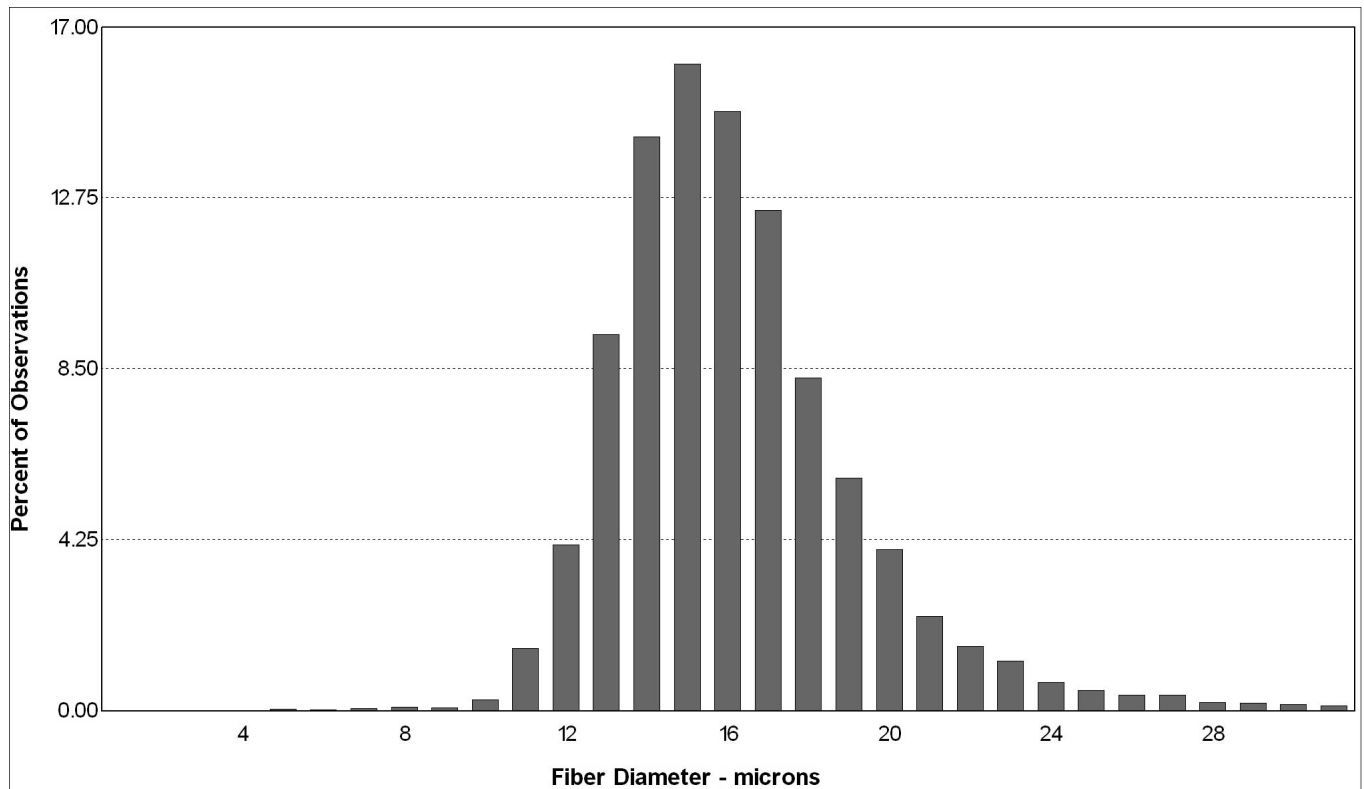

This Test Performed According to I.W.T.O Method 47