



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Brill Road
West Bolton QC J0E 2T0 Canada

Date: 07/12/19

Test No: 976948


Animal and Sample Description

Animal Name: Ariya Belenis' Anael
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: XXXXX
Sample Location: Mid Side
Sample Date: 05/05/19
Age: 08/27/17

Laboratory Data

Mean Fiber Diameter:	15.9 microns	Fibers Greater Than 30 microns:	0.4 %
Standard Deviation:	3.6 microns	Comfort Factor:	99.6 %
Coefficient of Variation:	22.9 %	Mean Curvature:	53.8 deg/mm
Spin Fineness:	15.8 microns	SD Curvature:	26.8 deg/mm

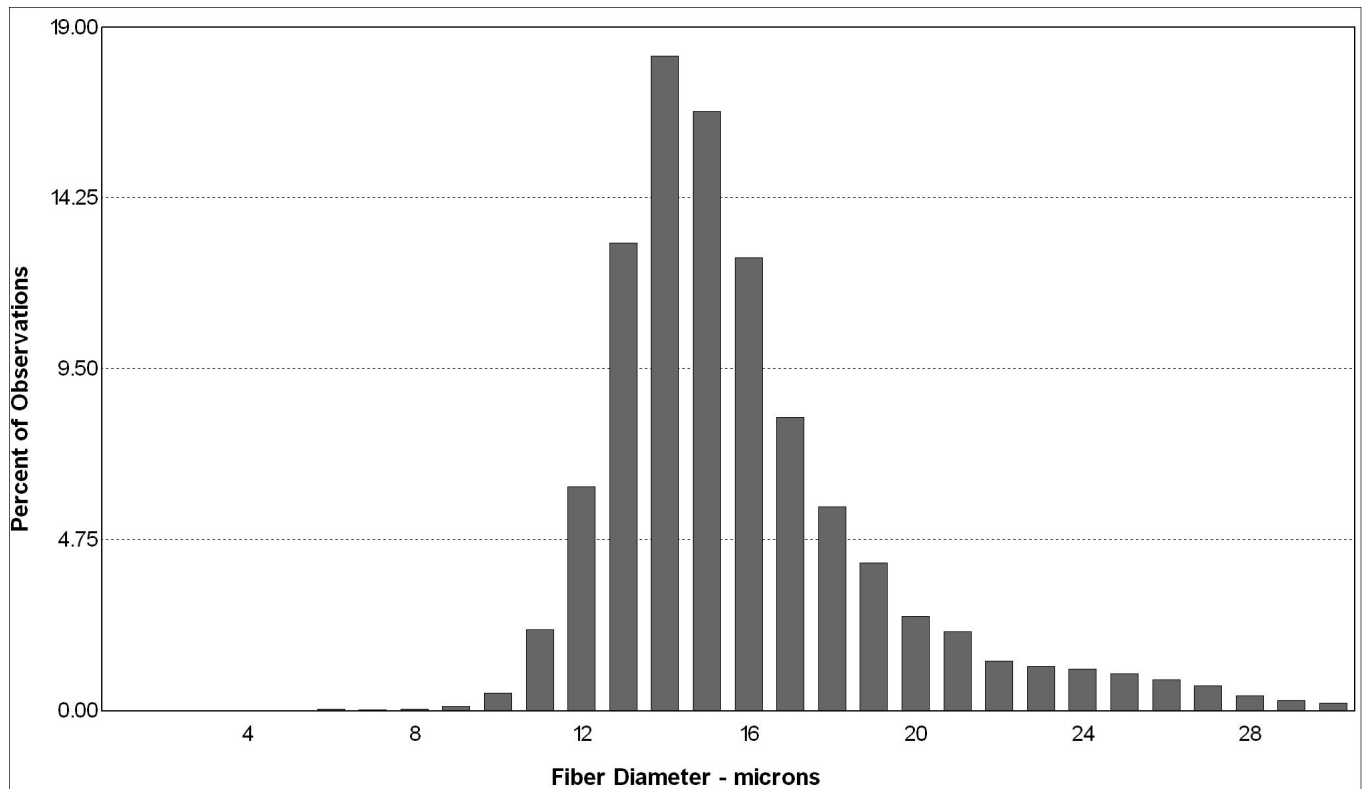

This Test Performed According to I.W.T.O Method 47