



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Ferme Criadorable/Nancy Bouchard  
177 Ch Poulin  
Dudswell QC J0B 2L0

10/11/17

Test No: 954307


### Animal and Sample Description

**Animal Name:** Criadorable Rebelle (999000001419573)  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Fawn

**Animal ID:** 44734  
**Sample Location:** Side  
**Sample Date:** 05/31/17  
**Age:** 07/29/12

### Laboratory Data

<b>Mean Fiber Diameter:</b>	22.4 microns	<b>Spin Fineness:</b>	22.7 microns
<b>Standard Deviation:</b>	5.6 microns	<b>Mean Curvature (deg/mm):</b>	42.0
<b>Coefficient of Variation:</b>	25.1 %	<b>SD Curvature (deg/mm):</b>	28.2
<b>Fibers Greater Than 30 microns:</b>	7.7 %	<b>Comfort Factor:</b>	92.3 %

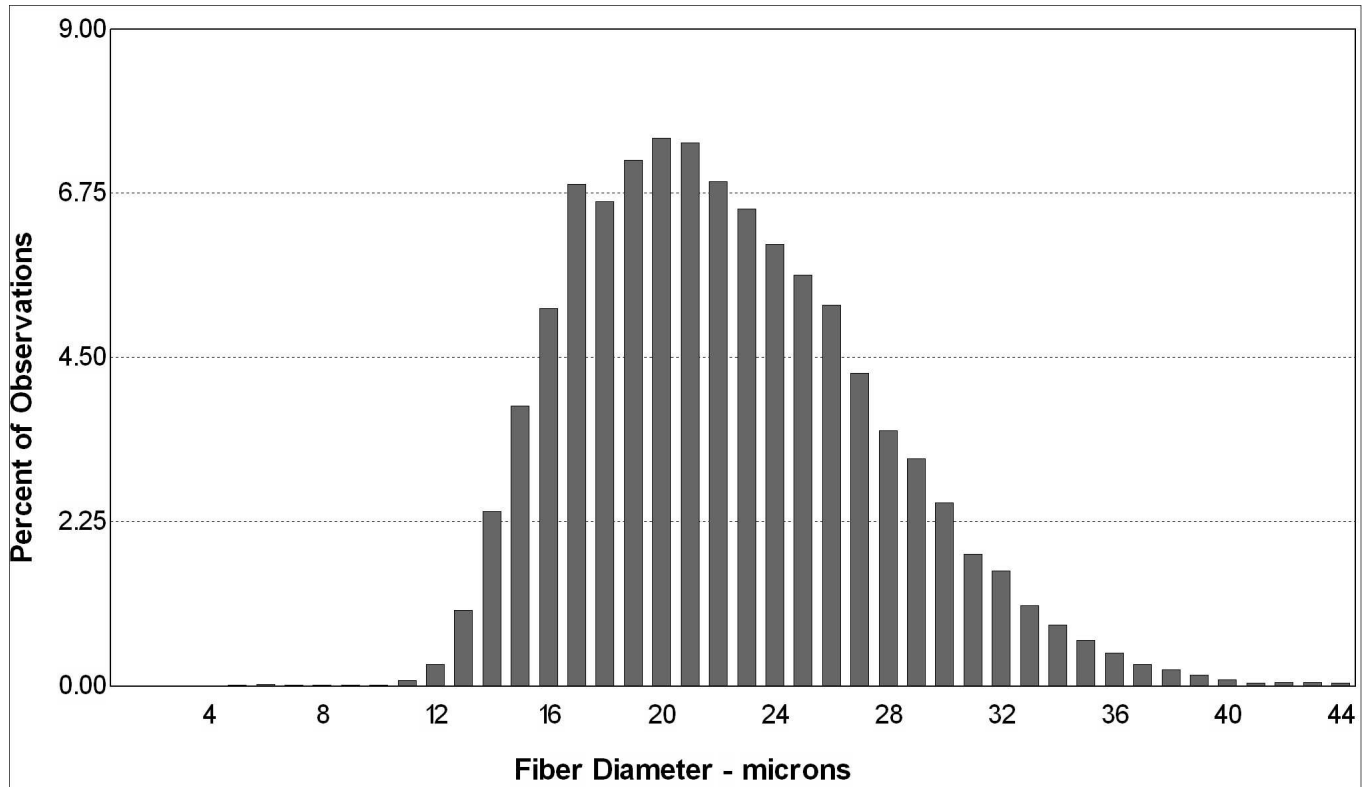

This Test Performed According to I.W.T.O Method 47