



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault  
411 Brill Road  
West Bolton QC J0E 2T0 Canada

**Date:** 07/12/19

**Test No:** 976980


### Animal and Sample Description

**Animal Name:** Ariya Salvations Simply White  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** White

**Animal ID:** 35562818  
**Sample Location:** Mid Side  
**Sample Date:** 05/05/19  
**Age:** 08/01/18

### Laboratory Data

<b>Mean Fiber Diameter:</b>	14.5 microns	<b>Fibers Greater Than 30 microns:</b>	0.7 %
<b>Standard Deviation:</b>	3.6 microns	<b>Comfort Factor:</b>	99.3 %
<b>Coefficient of Variation:</b>	24.6 %	<b>Mean Curvature:</b>	66.8 deg/mm
<b>Spin Fineness:</b>	14.6 microns	<b>SD Curvature:</b>	31.9 deg/mm

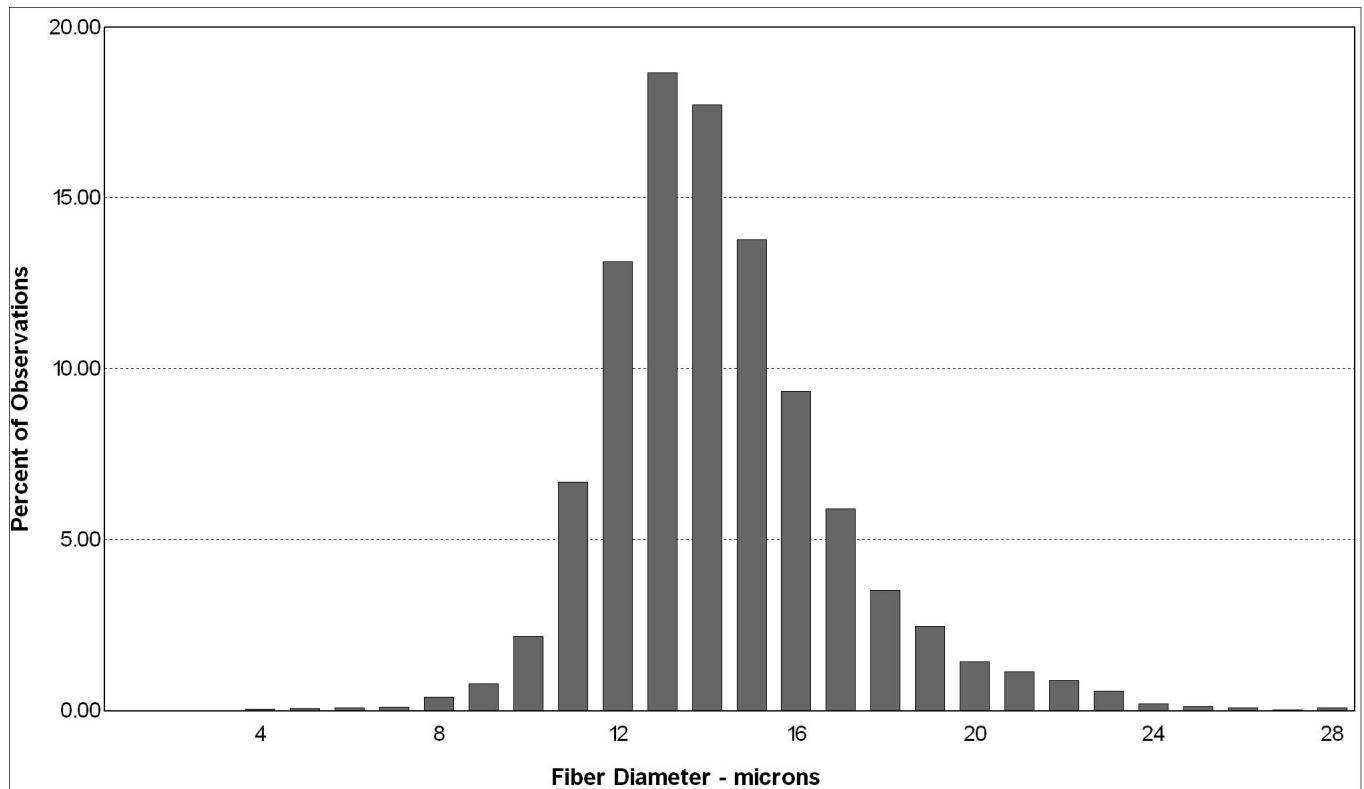

This Test Performed According to I.W.T.O Method 47