



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Brewster Alpacas/Kelly Brewster
Box 335
Bowden AB T0M 0K0 Canada

02/12/20

Test No: 987170


Animal and Sample Description

Animal Name: Olaveena Brew 956000008715104
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: 32763317
Sample Location: Side (L)
Sample Date: 05/10/19
Age: 06/24/13

Laboratory Data

Mean Fiber Diameter: 25.1 microns
Standard Deviation: 5.3 microns
Coefficient of Variation: 21.1 %
Fibers Greater Than 30 microns: 15.0 %

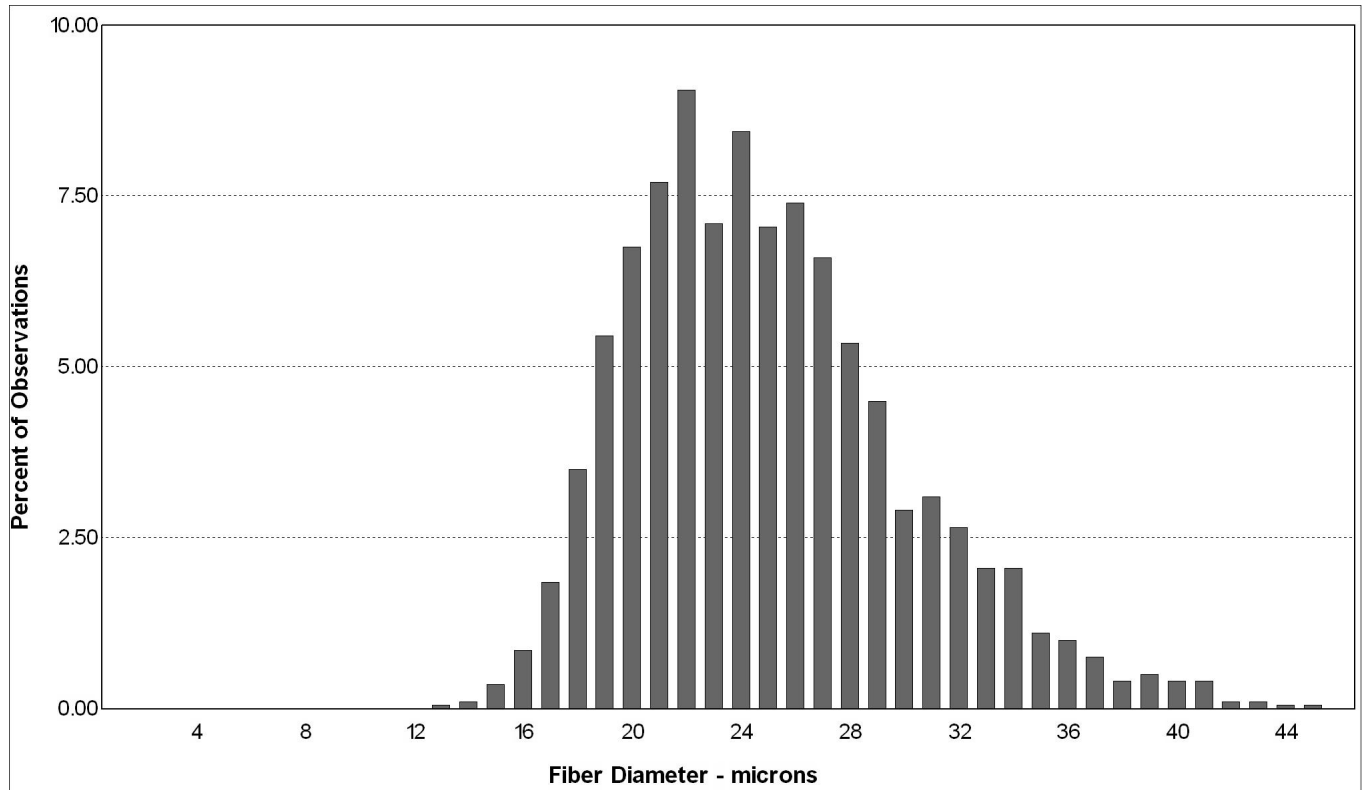

This Test Performed According to I.W.T.O Method 12