



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Hy-Haven Farm/Debby Filer
516 Johnson Hollow Rd
Cuba NY 14727-9610

Date: 07/26/16

Test No: 926042


Animal and Sample Description

Animal Name: Hy-Haven Absolute's Annistyn
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: 35064084
Sample Location: Side
Sample Date: 05/19/16
Age: 06/29/15

Laboratory Data

Mean Fiber Diameter:	15.2 microns	Fibers Greater Than 30 microns:	1.0 %
Standard Deviation:	4.1 microns	Comfort Factor:	99.0 %
Coefficient of Variation:	27.3 %	Mean Curvature:	54.5 deg/mm
Spin Fineness:	15.7 microns	SD Curvature:	32.5 deg/mm

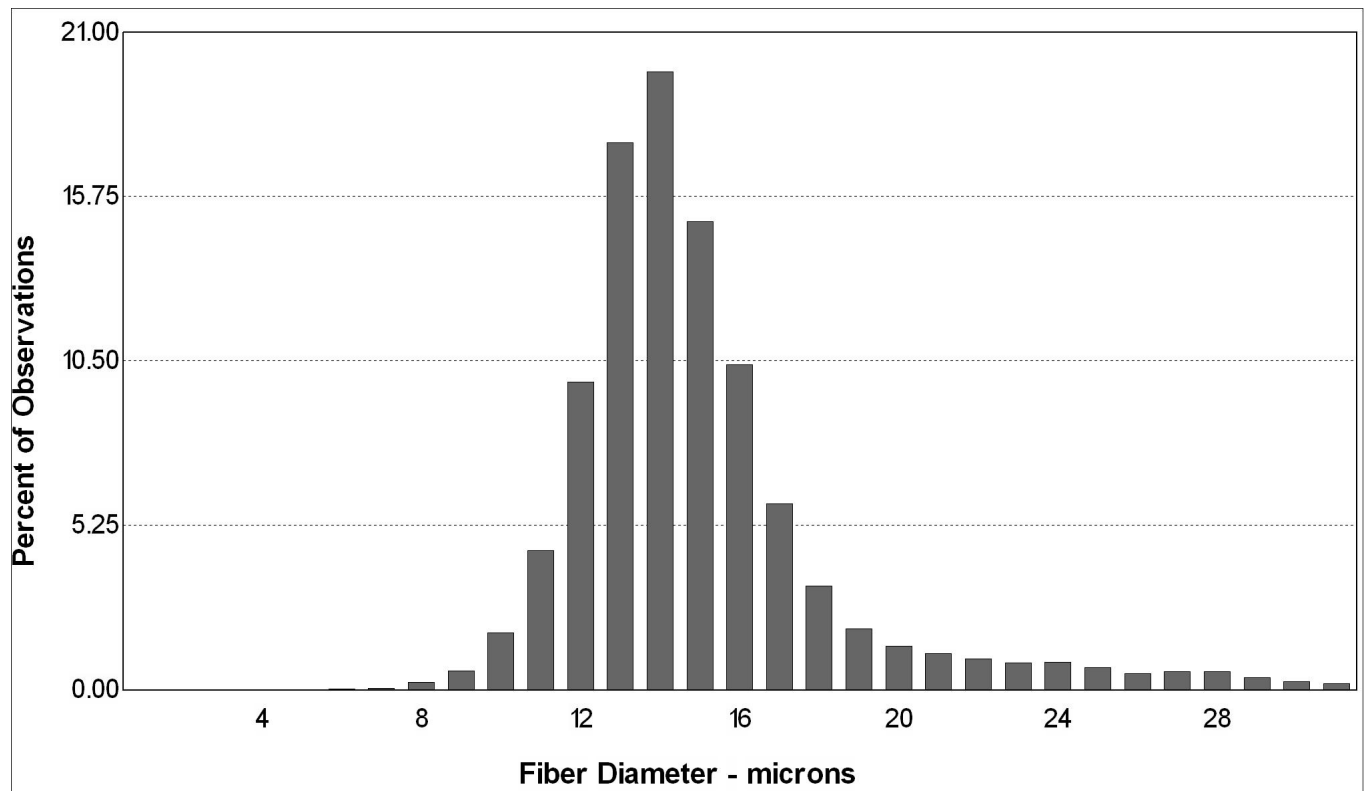

This Test Performed According to I.W.T.O Method 47