



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Pacesetter Alpacas/Dennis & Christy Pace
5546 W Plymouth Church Rd
Beloit WI 53511 USA

09/15/16

Test No: 935192


Animal and Sample Description

Animal Name: Copperfield
Breed: Alpaca(Suri)
Sex: Male
Color: Dark Fawn

Animal ID: 31581738
Sample Location: Mid Side
Sample Date: 05/01/16
Age: 06/12/13

Laboratory Data

Mean Fiber Diameter: 24.5 microns
Standard Deviation: 5.3 microns
Coefficient of Variation: 21.6 %
Fibers Greater Than 30 microns: 10.4 %

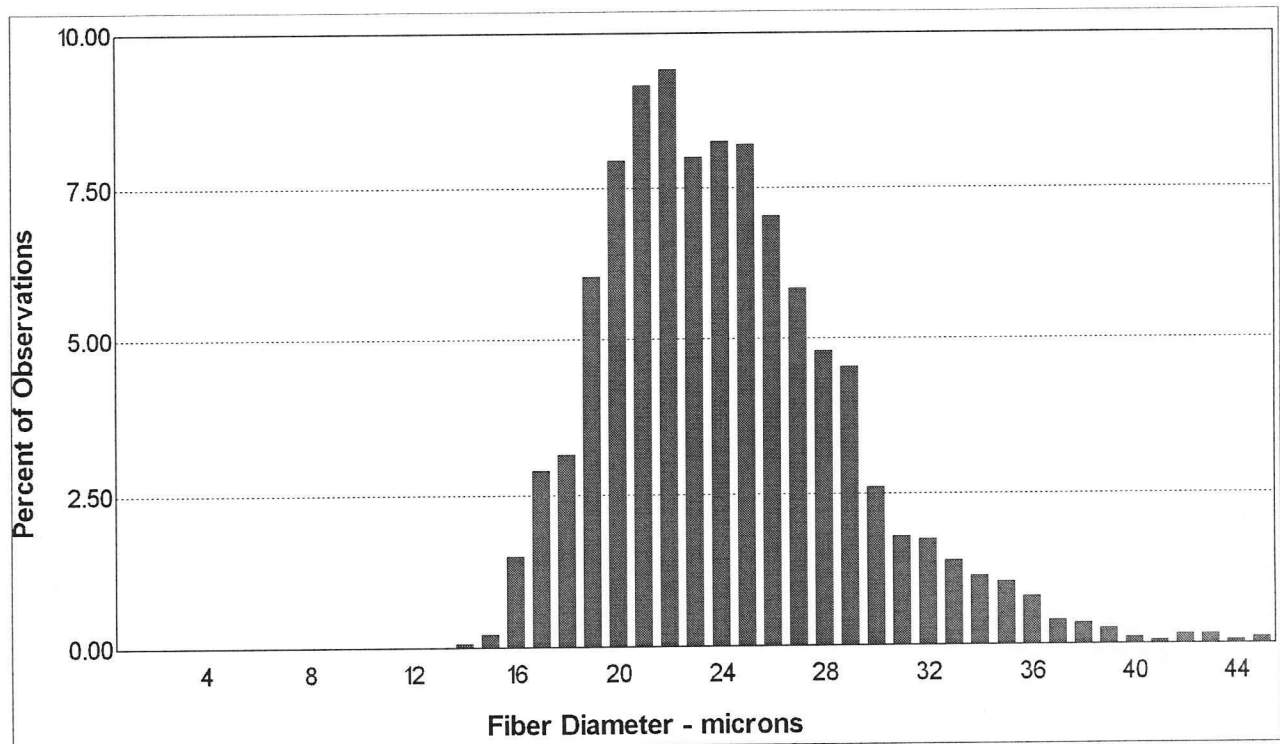

This Test Performed According to I.W.T.O Method 12



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Pacesetter Alpacas/Dennis Pace
5546 W Plymouth Church Rd
Beloit WI 53511 USA

09/03/15

Test No: 913796


Animal and Sample Description

Animal Name: Copper
Breed: Alpaca(Suri)
Sex: Male
Color: Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/23/15
Age: 06/12/13

Laboratory Data

Mean Fiber Diameter: 22.2 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 20.3 %
Fibers Greater Than 30 microns: 4.3 %

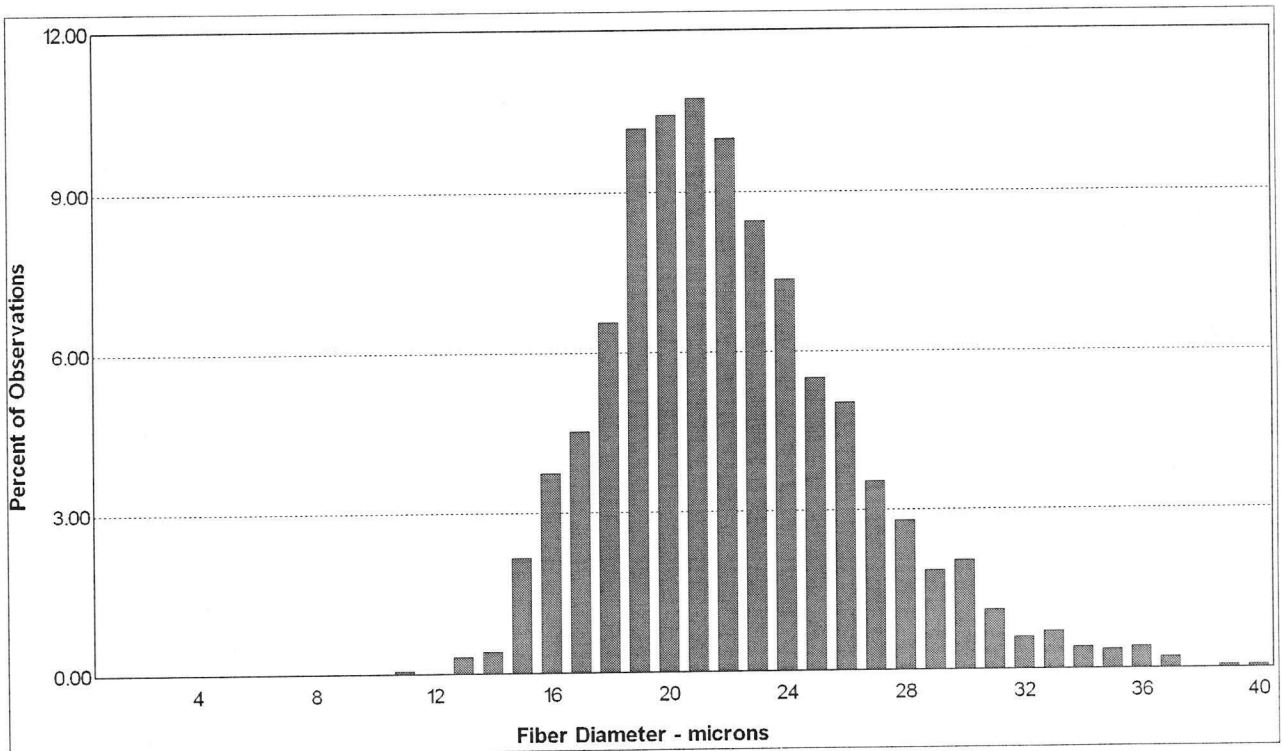

This Test Performed According to I.W.T.O Method 12



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Pacesetter Alpacas/Dennis Pace
5546 W Plymouth Church Rd
Beloit WI 53511 USA

08/22/14

Test No: 491545


Animal and Sample Description

Animal Name: Copperfield
Breed: Alpaca(Suri)
Sex: Male
Color: Dark Fawn

Animal ID: 31581738
Sample Location: Mid Side
Sample Date: 05/09/14
Age: 06/12/13

Laboratory Data

Mean Fiber Diameter: 17.8 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 25.2 %
Fibers Greater Than 30 microns: 1.7 %

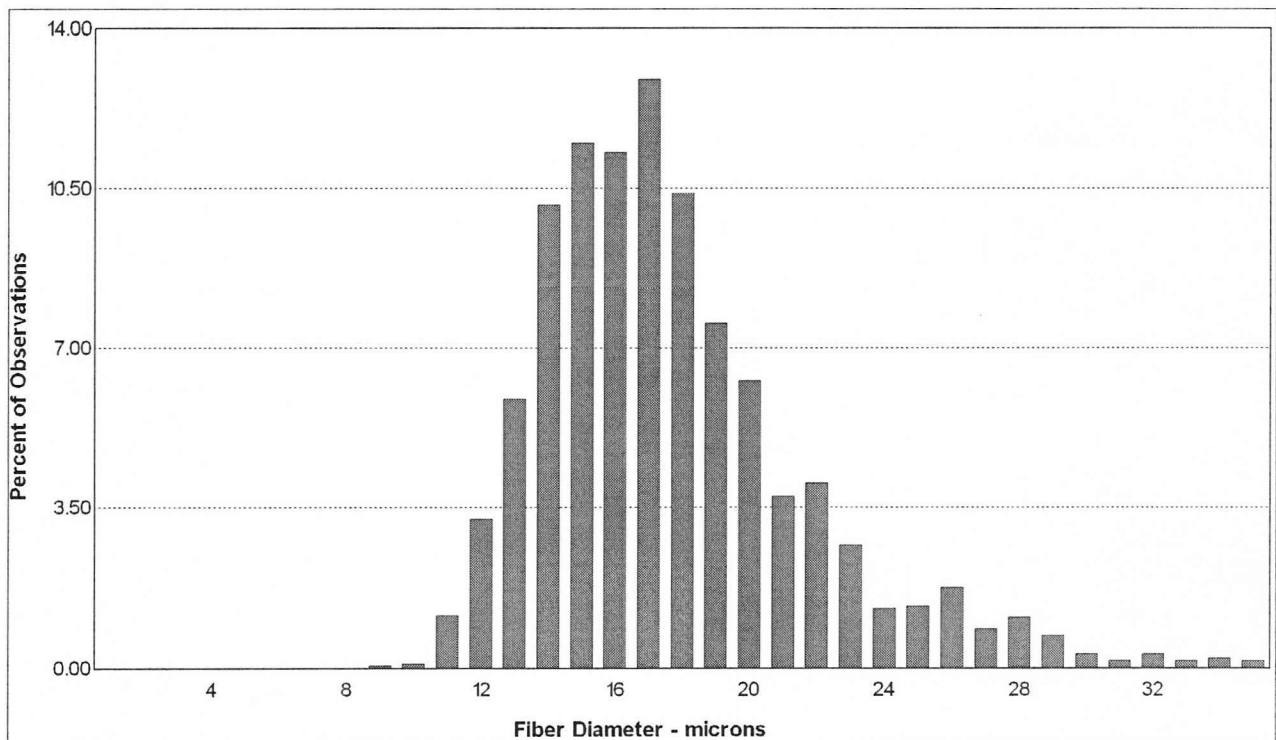

This Test Performed According to I.W.T.O Method 12