



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

B I Bar Ranch/Ted & Julie Ritschard  
8720 Moss Rock Rd  
Colorado Springs CO 80908 USA

07/22/19

Test No: 978591


### Animal and Sample Description

**Animal Name:** Durango  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** MRG

**Animal ID:** 35410867  
**Sample Location:** Mid Side  
**Sample Date:** 05/27/19  
**Age:** 06/17/17

### Laboratory Data

**Mean Fiber Diameter:** 23.5 microns  
**Standard Deviation:** 5.6 microns  
**Coefficient of Variation:** 23.7 %  
**Fibers Greater Than 30 microns:** 10.5 %

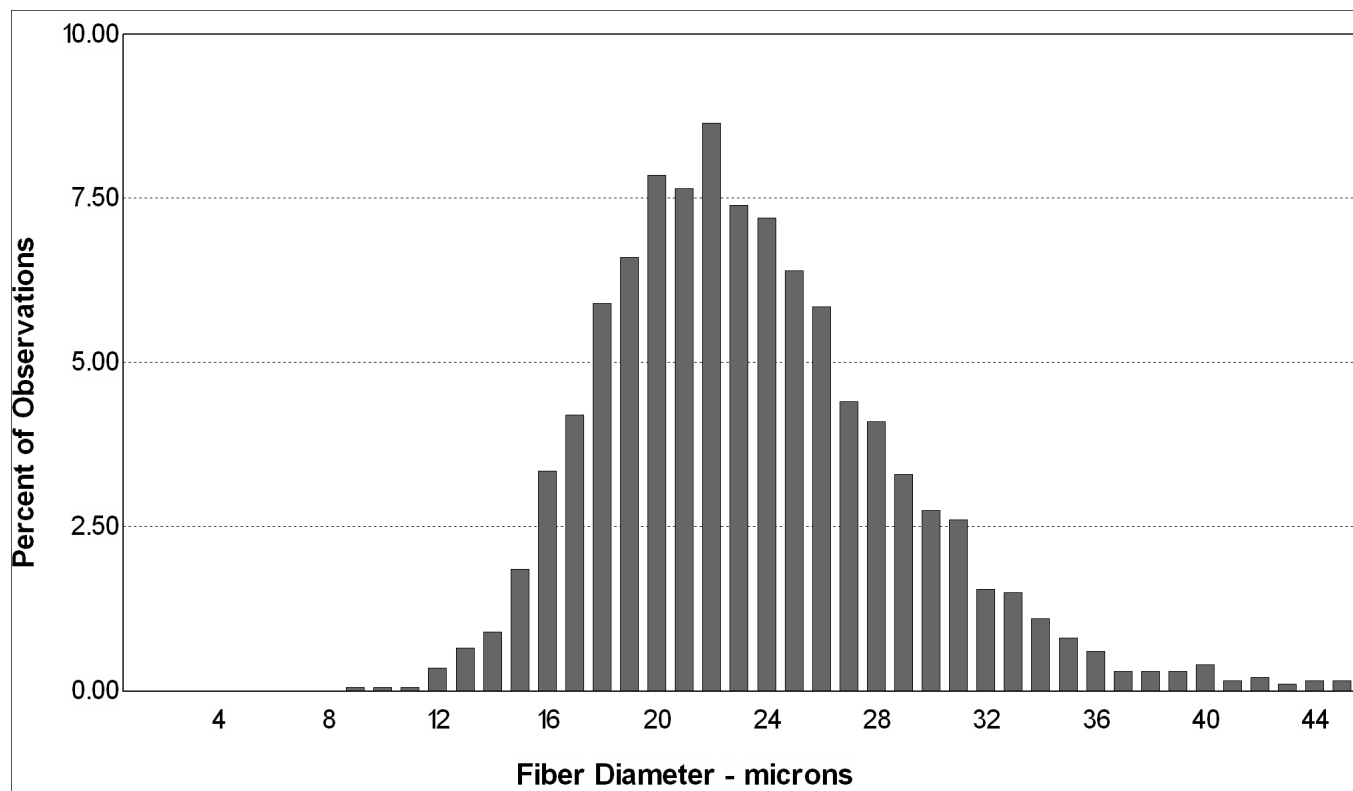

This Test Performed According to I.W.T.O Method 12