



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

B I Bar Ranch/Julie Ritschard  
8720 Moss Rock Rd  
Colorado Springs CO 80908 USA

06/24/13

Test No: 458373


### Animal and Sample Description

**Animal Name:** Gunnison  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Black

**Animal ID:** 31622165  
**Sample Location:** Side (R)  
**Sample Date:** 05/30/13  
**Age:** 07/17/09

### Laboratory Data

**Mean Fiber Diameter:** 23.8 microns  
**Standard Deviation:** 6.8 microns  
**Coefficient of Variation:** 28.8 %  
**Fibers Greater Than 30 microns:** 14.5 %

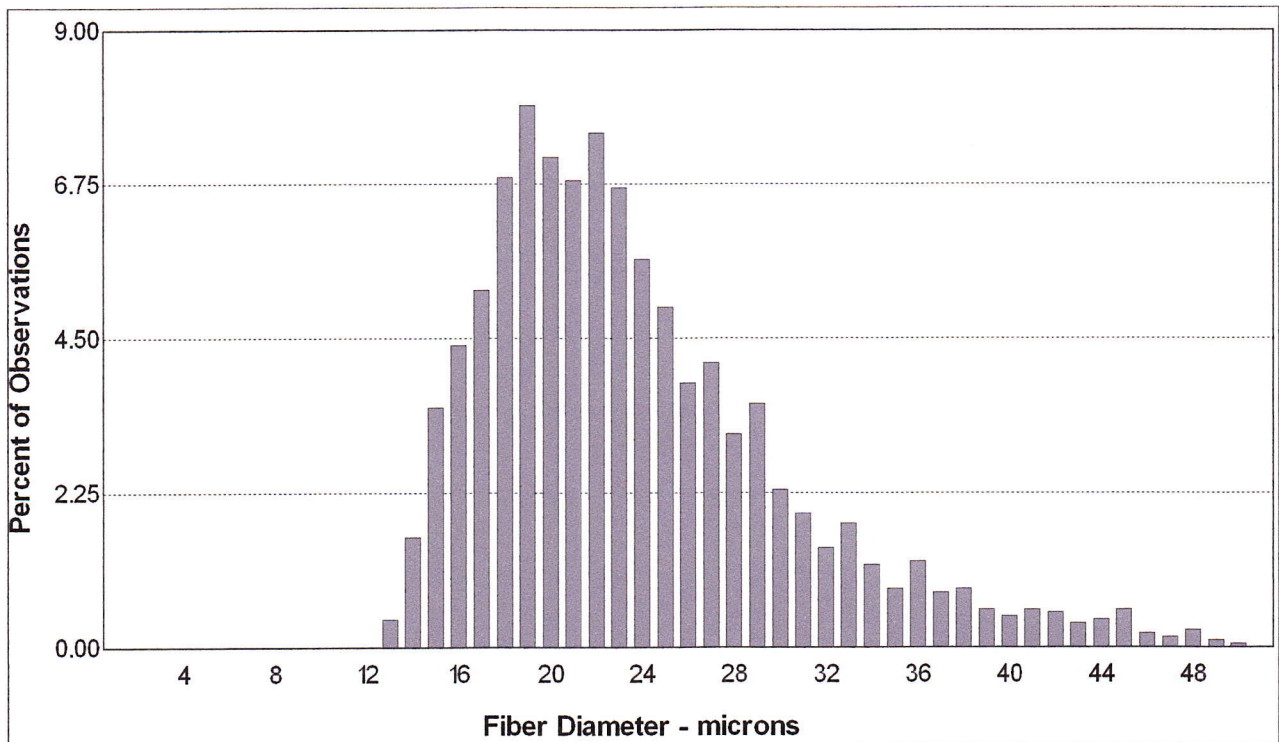

This Test Performed According to I.W.T.O Method 12