

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

B I Bar Ranch/Julie M Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

06/16/18

Test No: 961874


Animal and Sample Description

Animal Name: BIR's Hesperus
Breed: Alpaca(Suri)
Sex: Male
Color: MF

Animal ID: 35198703
Sample Location: Side (R)
Sample Date: 06/01/18
Age: 07/26/17

Laboratory Data

Mean Fiber Diameter: 19.1 microns
Standard Deviation: 3.8 microns
Coefficient of Variation: 19.9 %
Fibers Greater Than 30 microns: 0.7 %

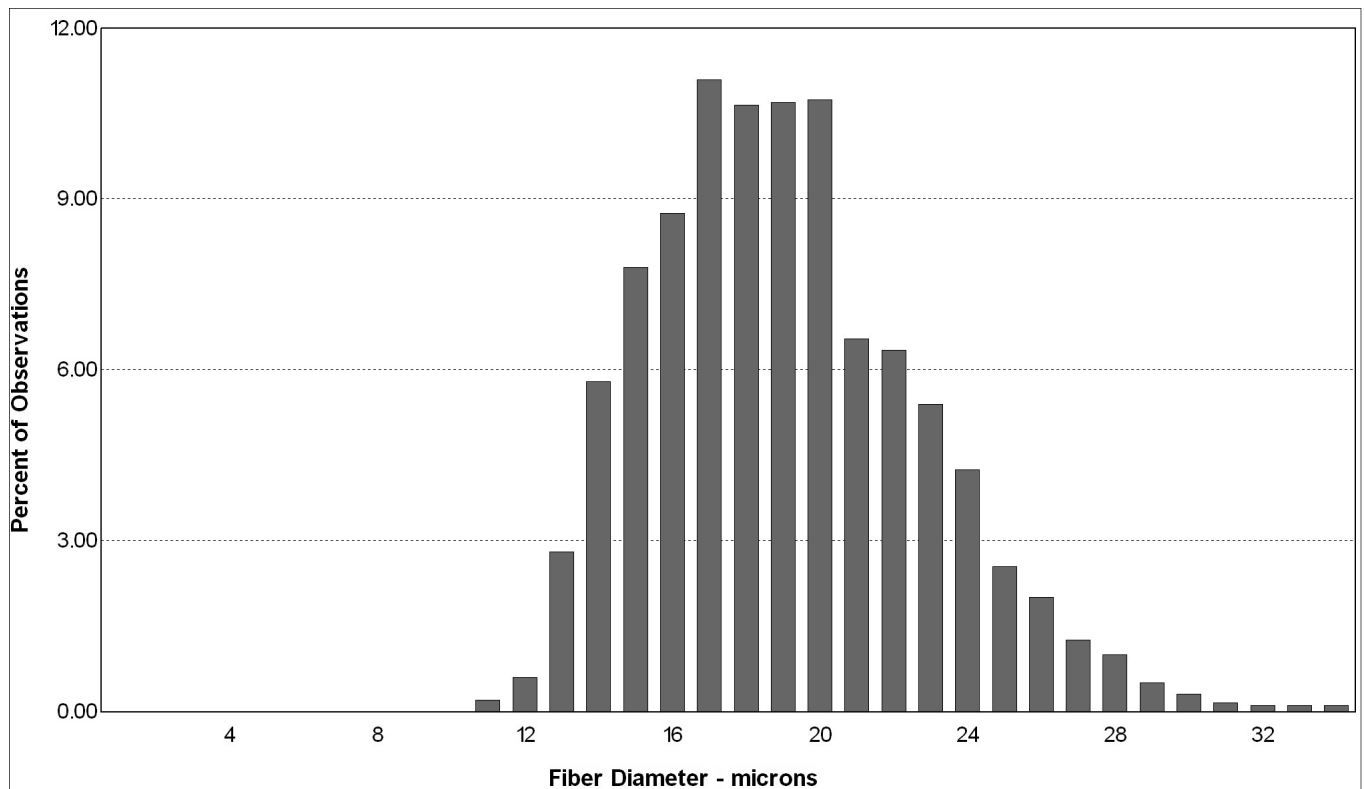

This Test Performed According to I.W.T.O Method 12