

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

B I Bar Ranch/Julie Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

07/16/12

Test No: 435560


Animal and Sample Description

Animal Name: Keystone
Breed: Alpaca(Suri)
Sex: Male
Color: Beige

Animal ID: 31831796
Sample Location: Side
Sample Date: 05/30/12
Age: 11/01/11

Laboratory Data

Mean Fiber Diameter: 22.9 microns
Standard Deviation: 4.6 microns
Coefficient of Variation: 20.0 %
Fibers Greater Than 30 microns: 3.8 %

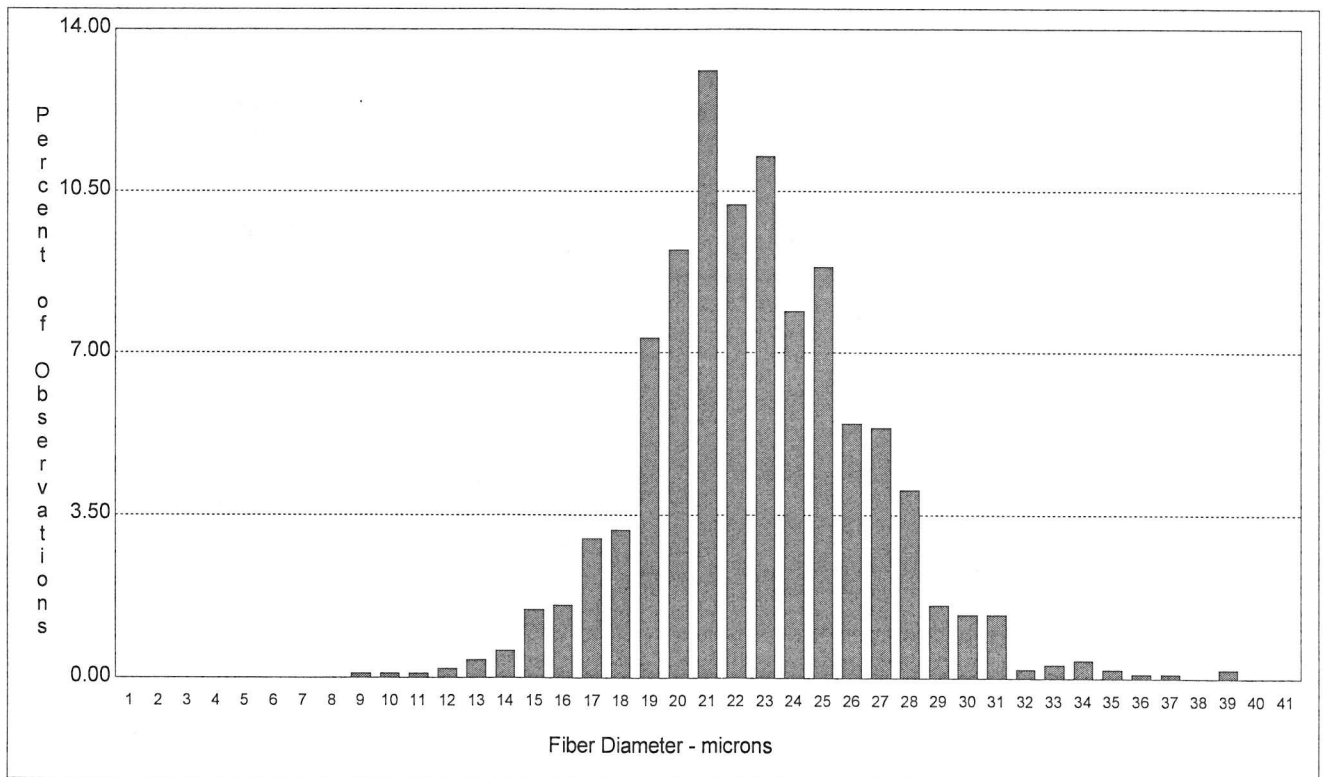

This Test Performed According to I.W.T.O Method 12