



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

B I Bar Ranch/Ted & Julie Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

07/22/19

Test No: 978597


Animal and Sample Description

Animal Name: BIR's Nelson
Breed: Alpaca(Suri)
Sex: Male
Color: MRG

Animal ID: XXXXX
Sample Location: Mid Side
Sample Date: 05/27/19
Age: 06/06/16

Laboratory Data

Mean Fiber Diameter: 22.4 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 20.3 %
Fibers Greater Than 30 microns: 4.7 %

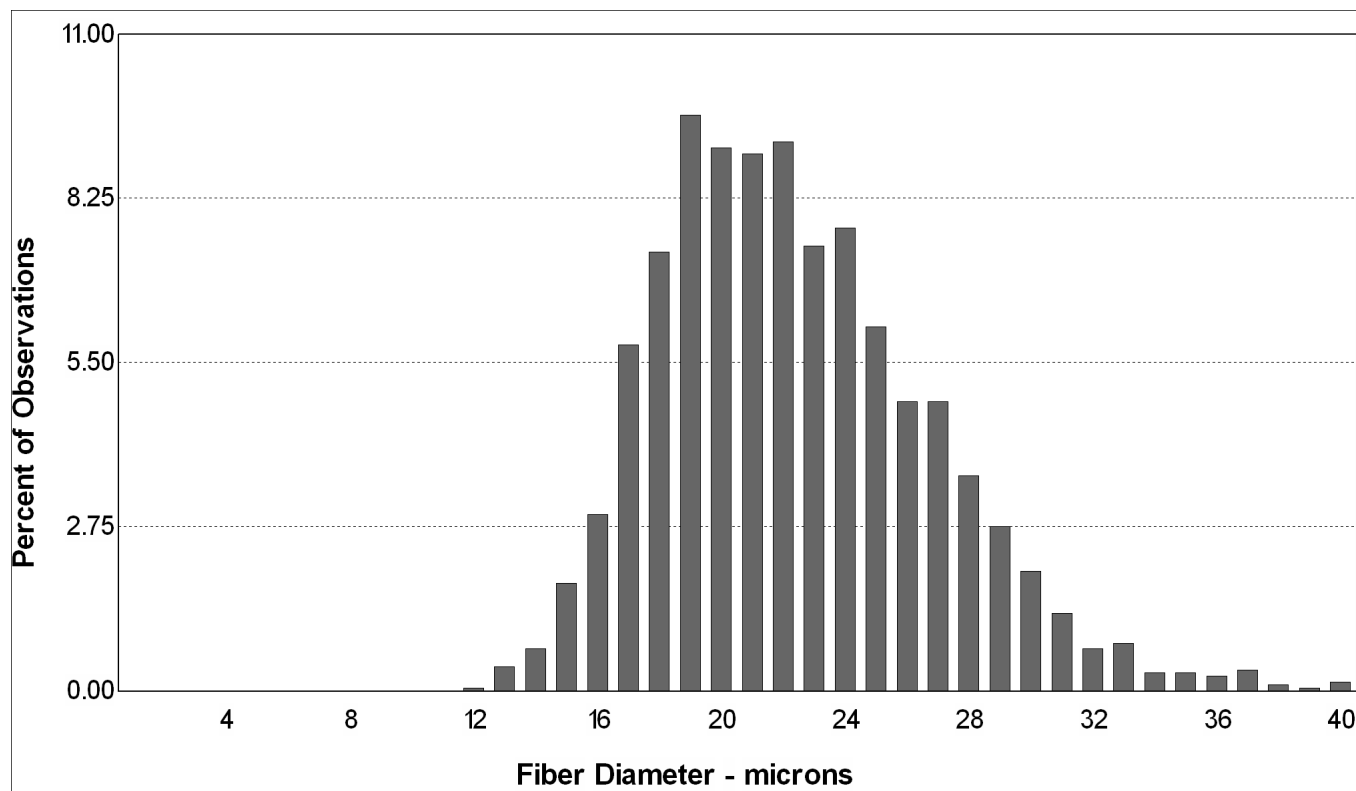

This Test Performed According to I.W.T.O Method 12