

Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Glengary Farm Alpacas/Patrick J. Cassese
2078 Glengary Road
Akron OH 44333 U.S.A.

06/08/07

Test No: 297106


Animal and Sample Description

Animal Name: Double Deuce PLA
Breed: Alpaca(Huacaya)
Sex: Male
Color: Black

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/29/07
Age: 05/25/05

Laboratory Data

Mean Fiber Diameter: 20.5 microns
Standard Deviation: 4.1 microns
Coefficient of Variation: 20.0 %
Fibers Greater Than 30 microns: 2.3 %

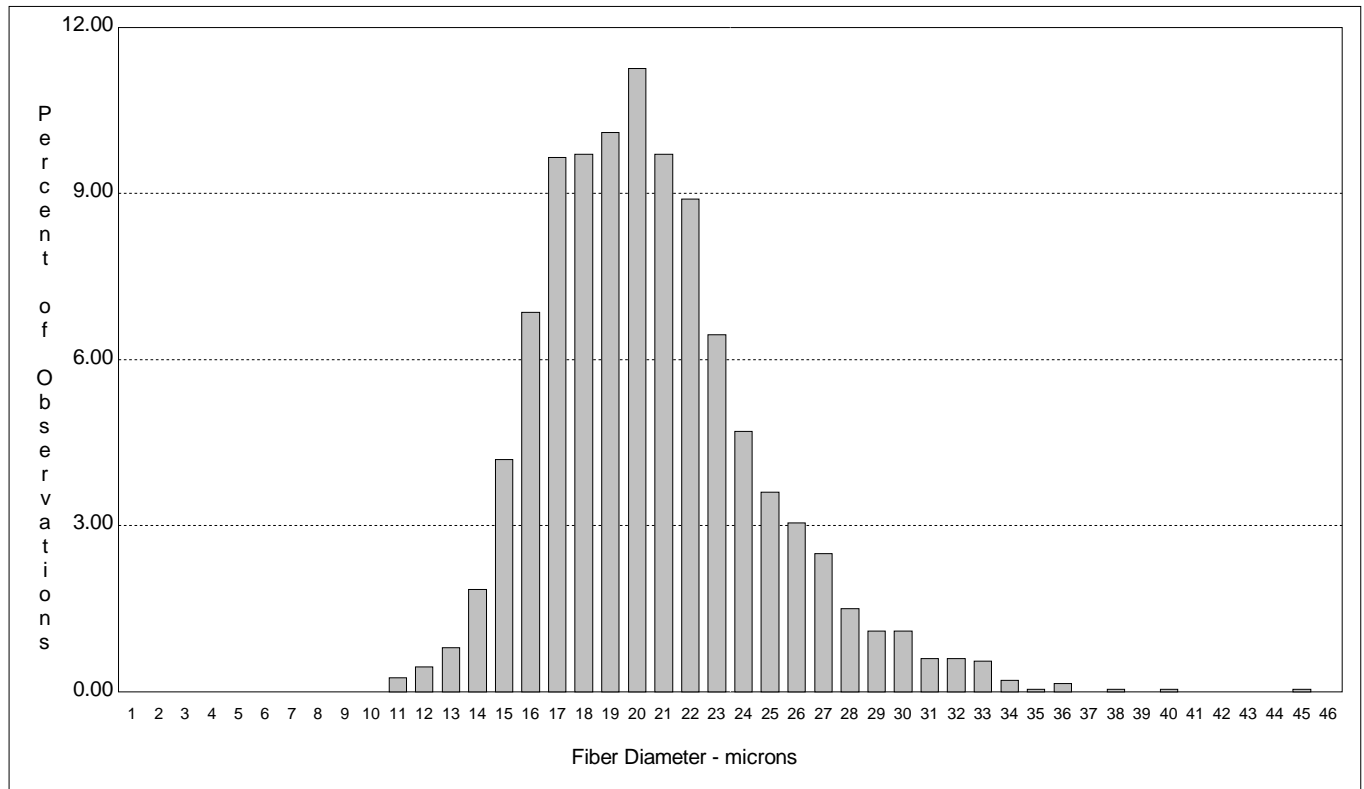

This Test Performed According to I.W.T.O Method 12