



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Peruvian Soul Alpaca Farm/Dr. Luis G. Iturriaga
5939 Market Avenue North
Canton OH 44721-3234 USA

08/20/08

Test No: 333396


Animal and Sample Description

Animal Name: Perusoul Peruvian Shazaam's Misti
Breed: Alpaca(Huacaya)
Sex: Male
Color: Light Fawn

Animal ID: 30848207
Sample Location: Side
Sample Date: 04/17/08
Age: 09/14/07

Laboratory Data

Mean Fiber Diameter: 21.1 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 21.3 %
Fibers Greater Than 30 microns: 3.1 %

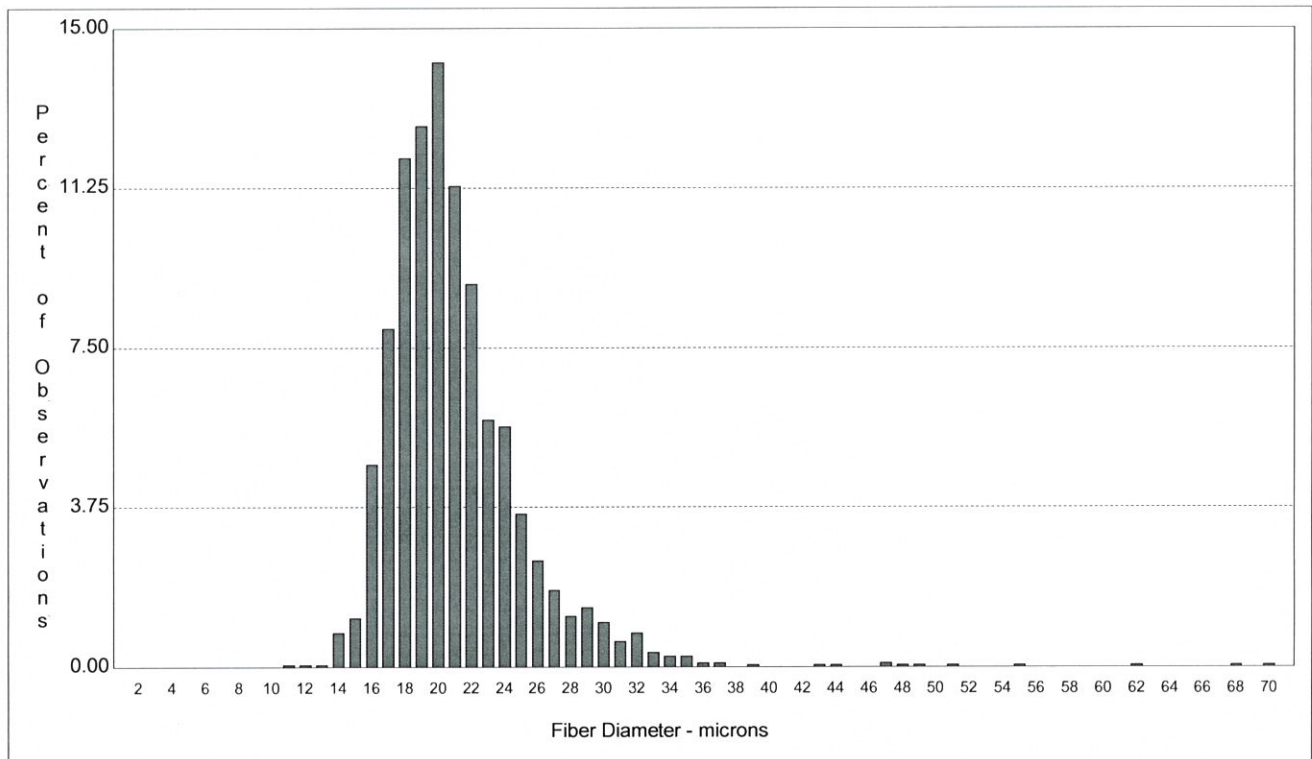

This Test Performed According to I.W.T.O Method 12