



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Peruvian Soul Alpaca Farm/Dr. Luis G. Iturriaga
8011 Chatham Rd
Medina OH 44256-9171 USA

09/26/14

Test No: 493429


Animal and Sample Description

Animal Name: SSF Accoyo Eduardo (2011)
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: 31975827
Sample Location: Mid Side
Sample Date: 05/16/11
Age: 04/18/10

Laboratory Data

Mean Fiber Diameter: 12.8 microns
Standard Deviation: 2.5 microns
Coefficient of Variation: 19.3 %
Fibers Greater Than 30 microns: 0.2 %

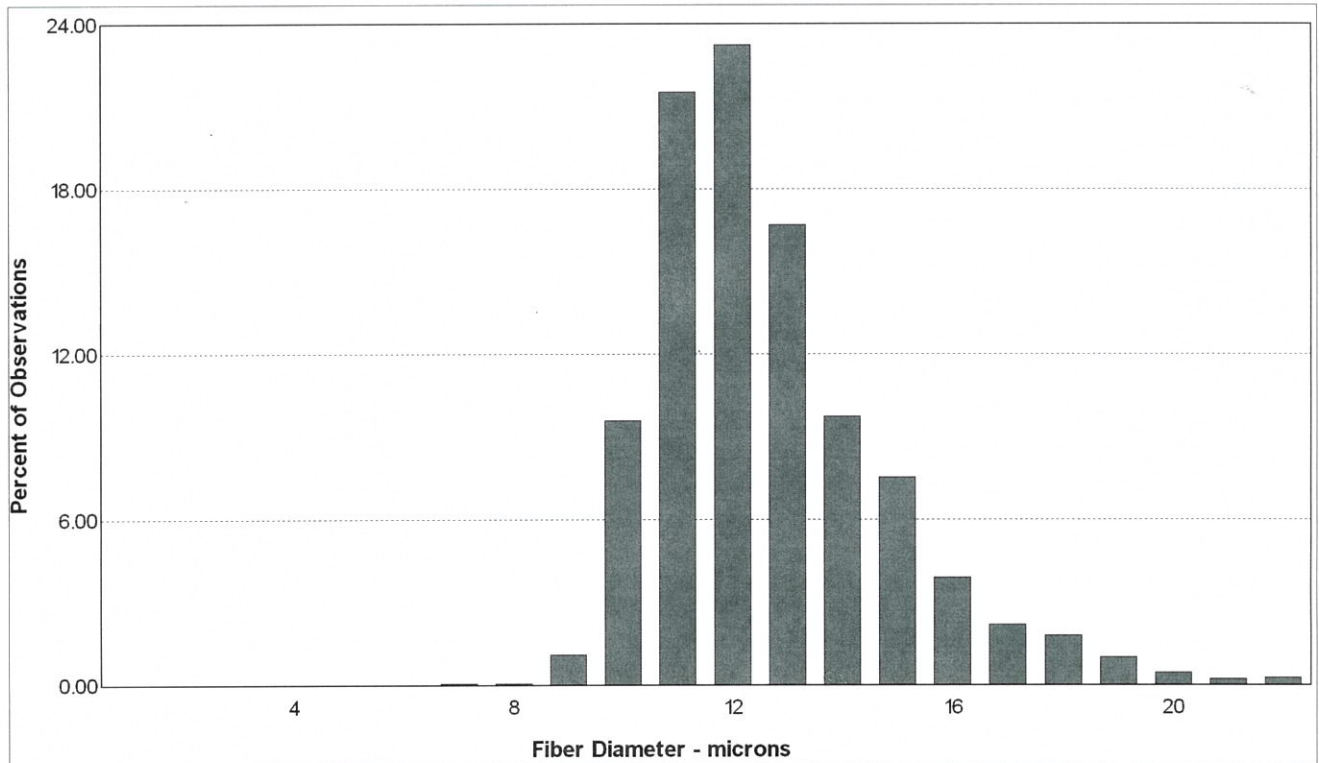

This Test Performed According to I.W.T.O Method 12