

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan  
Micron Test Report

Stachowski Alpacas, LLC/Anthony Stachowski DVM  
P.O. Box 828  
Mantua OH 44255

07/31/15

Test No: 909939


## Animal and Sample Description

Animal Name: 87  
Breed: Alpaca(Huacaya)  
Sex: Male  
Color: W

Animal ID: 87  
Sample Location: Side  
Sample Date: 05/16/14  
Age: 06/07/13

## Laboratory Data

Mean Fiber Diameter: 16.5 microns  
Standard Deviation: 2.9 microns  
Coefficient of Variation: 17.8 %  
Fibers Greater Than 30 microns: 0.5 %

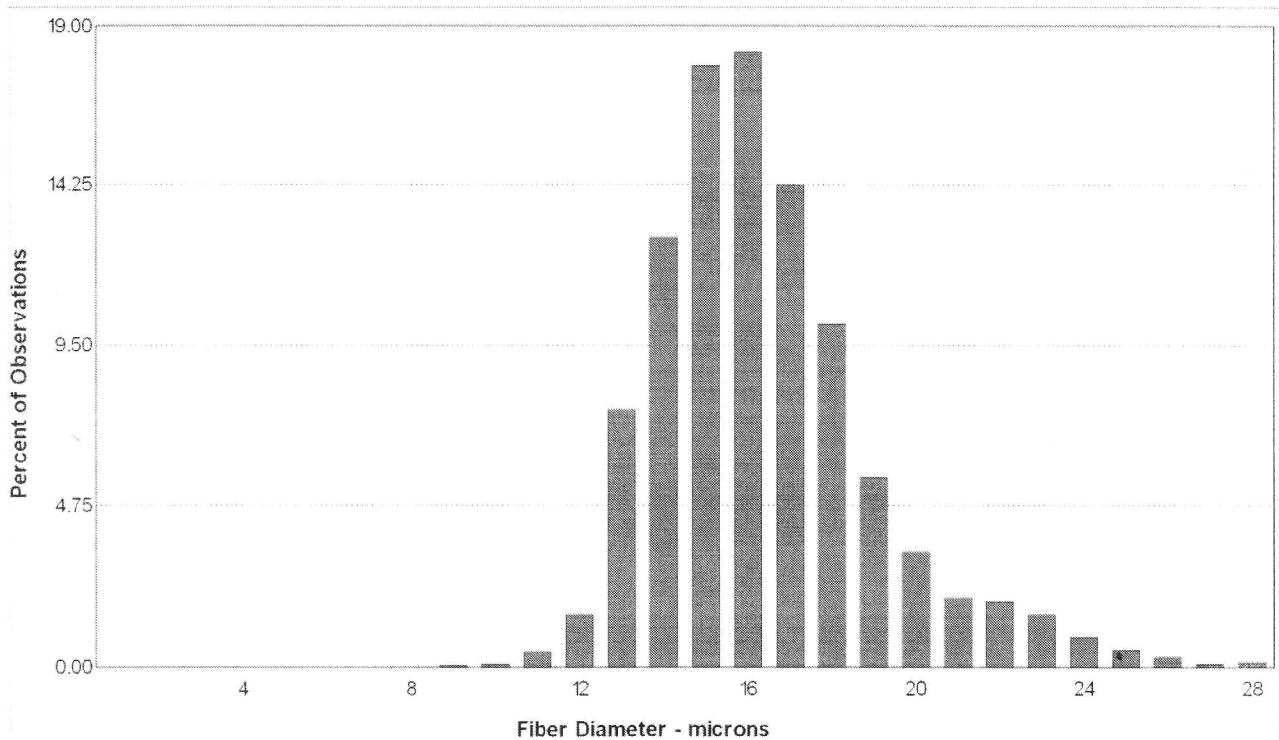

This Test Performed According to I.W.T.O Method 12