



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Stachowski Alpacas, LLC/Anthony Stachowski DVM
12648 State Route 44
Mantua OH 44255

08/16/16

Test No: 931935


Animal and Sample Description

Animal Name: Royal Peruvian Light My Fire
Breed: Alpaca(Huacaya)
Sex: Female
Color: DB

Animal ID: 64
Sample Location: Side
Sample Date: 05/14/15
Age: 09/20/14

Laboratory Data

Mean Fiber Diameter: 16.7 microns
Standard Deviation: 4.2 microns
Coefficient of Variation: 25.4 %
Fibers Greater Than 30 microns: 2.2 %

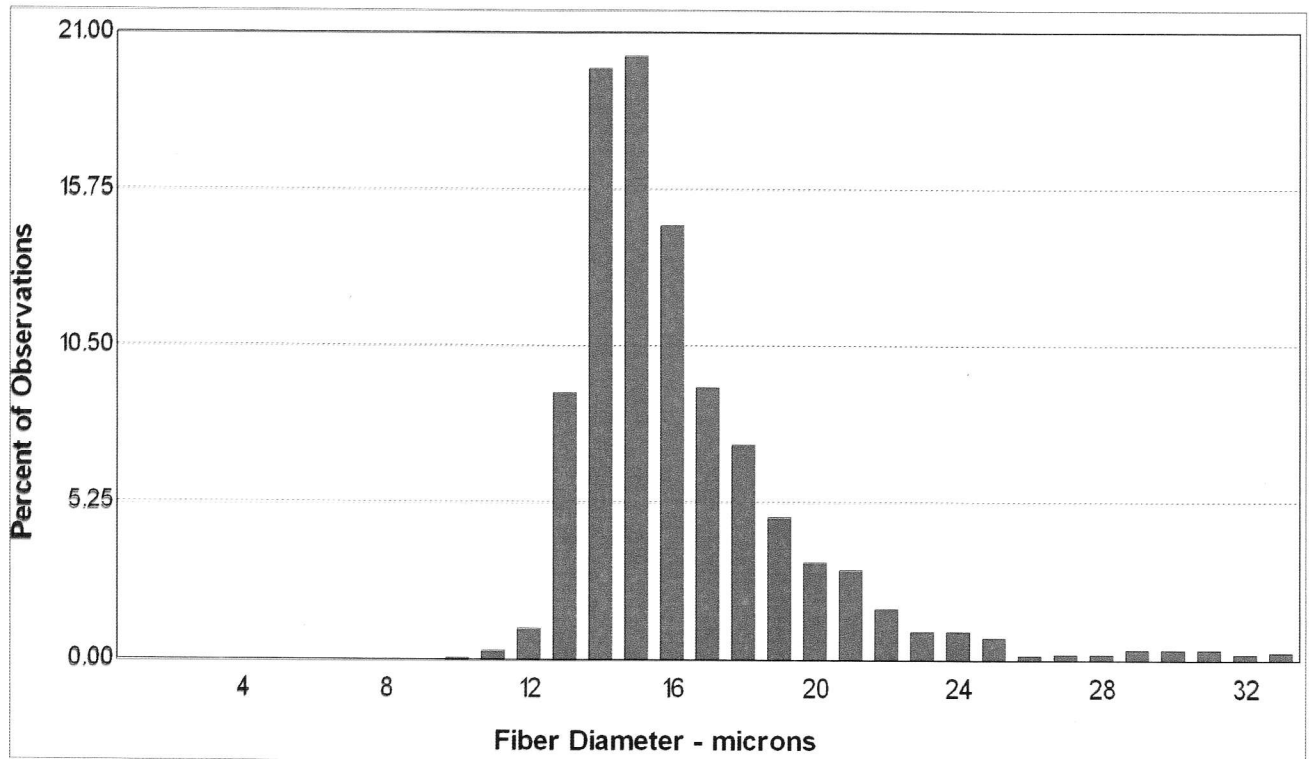

This Test Performed According to I.W.T.O Method 12