



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpacas of Moose Creek Ranch/Debbie Hoerl
23681 Quivira Road
Bucyrus KS 66013

Date: 06/19/19

Test No: 975927


Animal and Sample Description

Animal Name: Red Granite's Dusty
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Silver Grey

Animal ID: 35168621
Sample Location: Side
Sample Date: 04/23/2019
Age: 07/18/2015

Laboratory Data

Mean Fiber Diameter:	20.1 microns	Fibers Greater Than 30 microns:	4.0 %
Standard Deviation:	4.9 microns	Comfort Factor:	96.0 %
Coefficient of Variation:	24.3 %	Mean Curvature:	42.1 deg/mm
Spin Fineness:	20.2 microns	SD Curvature:	22.6 deg/mm

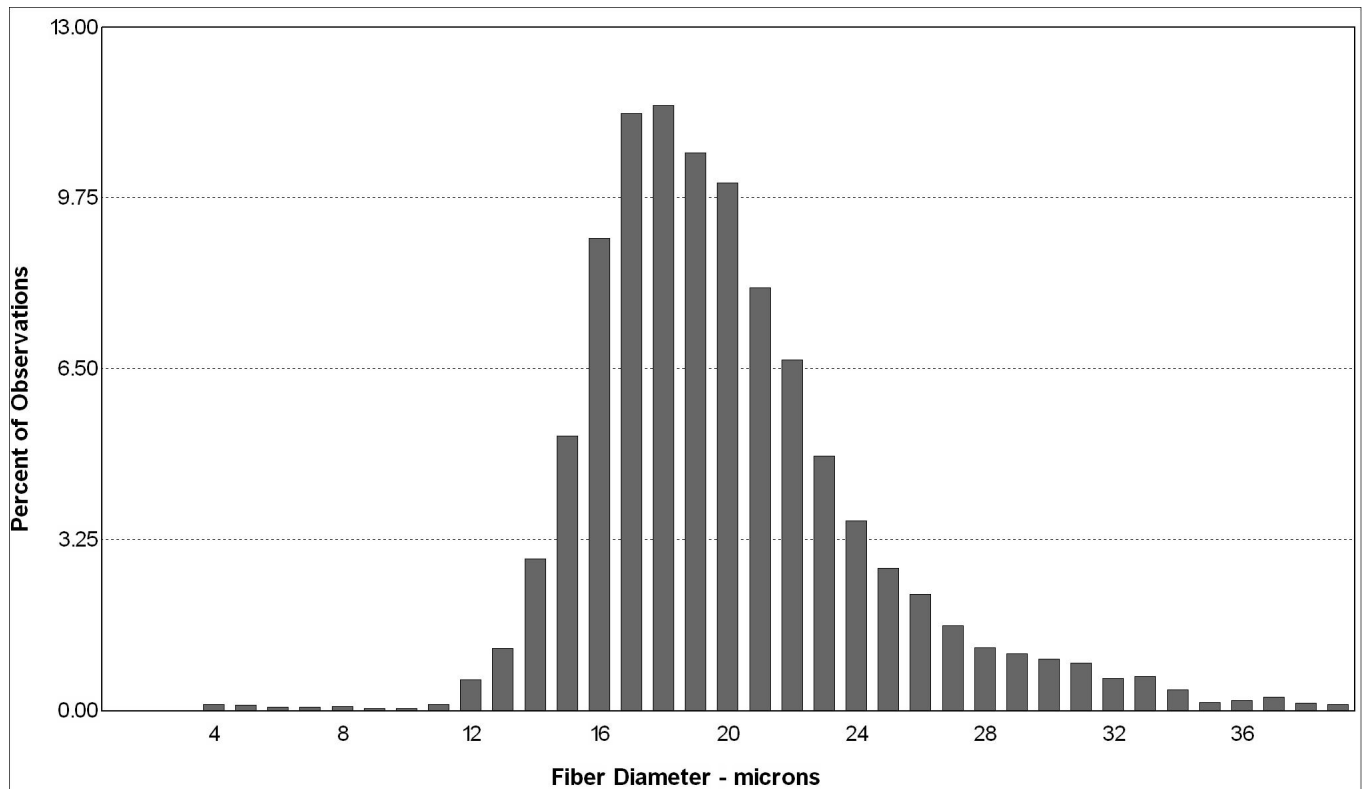

This Test Performed According to I.W.T.O Method 47