



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

West Penn Alpacas/M. Vigus & D. Harden-Vigus
1843 E. Finley Dr
Claysville PA 15323 USA

03/21/15

Test No: 498242


Animal and Sample Description

Animal Name: WP Vela by Verticase
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Brown

Animal ID: 32691559
Sample Location: Side (L)
Sample Date: 05/22/14
Age: 10/03/13

Laboratory Data

Mean Fiber Diameter: 15.4 microns
Standard Deviation: 2.6 microns
Coefficient of Variation: 16.8 %
Fibers Greater Than 30 microns: 0.2 %

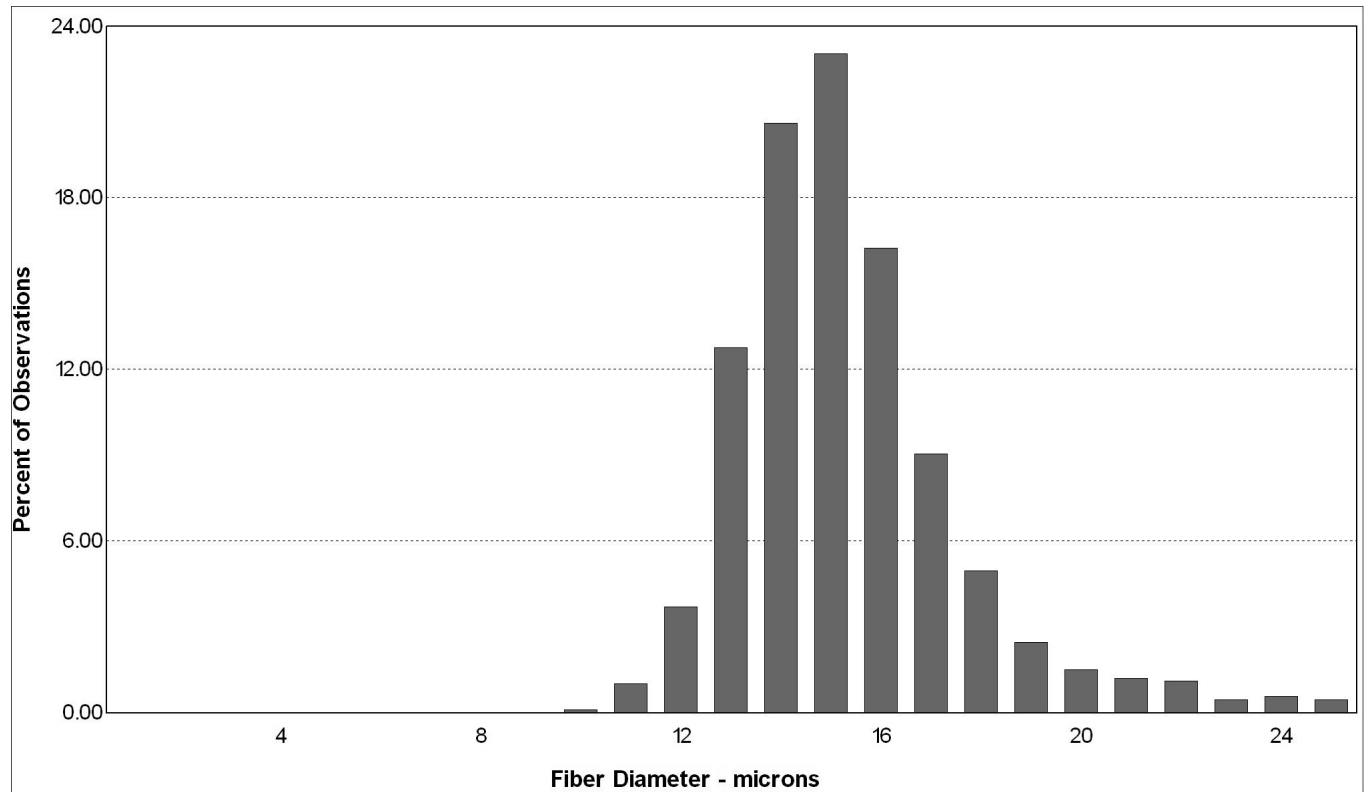

This Test Performed According to I.W.T.O Method 12