



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Baker's Alpaca Patch/Richard A. Veverka
5081 East Lake Rd
Jamestown PA 16134 USA

08/26/13

Test No: 467878


Animal and Sample Description

Animal Name: Charlie Remington
Breed: Alpaca(Suri)
Sex: Male
Color: Med Fawn

Animal ID: 32143928
Sample Location: Side
Sample Date: 05/24/13
Age: 08/06/11

Laboratory Data

Mean Fiber Diameter: 19.2 microns
Standard Deviation: 3.9 microns
Coefficient of Variation: 20.4 %
Fibers Greater Than 30 microns: 1.2 %

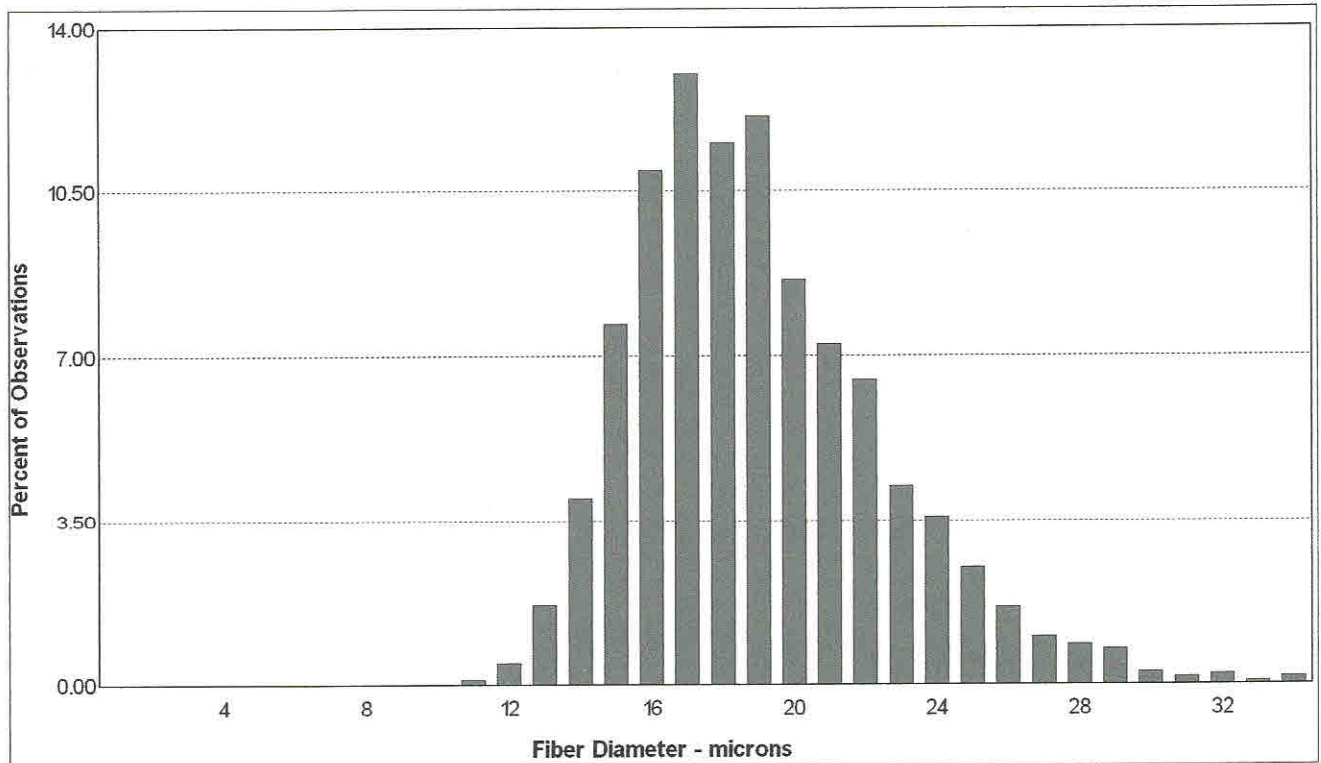

This Test Performed According to I.W.T.O Method 12