



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Alpacas of the Covenant, Inc/Kimberly Buechner Fouse
108 Ridgepointe Dr
Cold Spring KY 41076-9090

07/06/16

Test No: 925674


Animal and Sample Description

Animal Name: ACOV Peruvian Frango's Zuri
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Brown

Animal ID: 31705301
Sample Location: Side
Sample Date: 05/16/16
Age: 06/20/11

Laboratory Data

Mean Fiber Diameter: 21.8 microns
Standard Deviation: 3.8 microns
Coefficient of Variation: 17.3 %
Fibers Greater Than 30 microns: 3.7 %

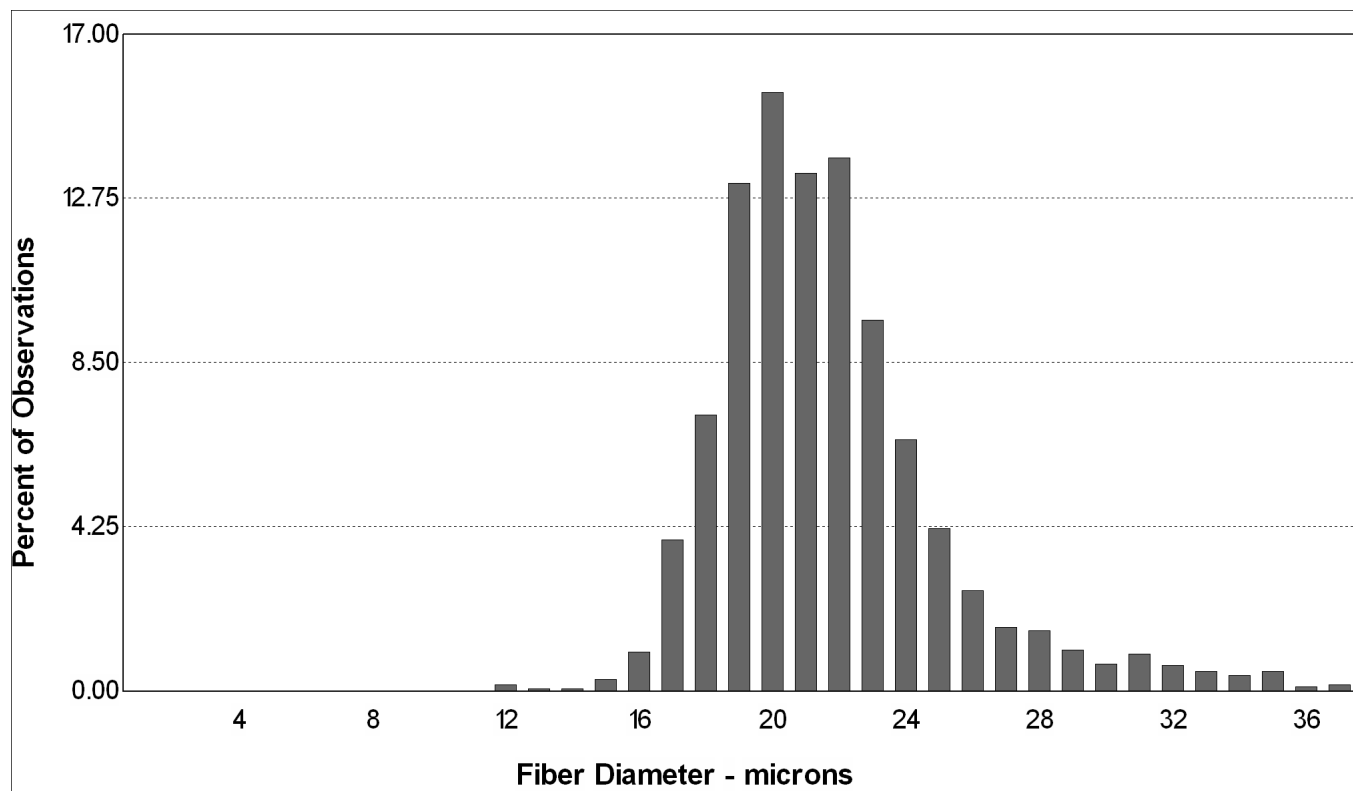

This Test Performed According to I.W.T.O Method 12