



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Glengary Farm Alpacas/Patrick Cassese  
2704 Slessman Drive  
Plymouth OH 44865 USA

**Date:** 07/03/18

**Test No:** 962517


### Animal and Sample Description

**Animal Name:** GGF Accoyo Avery's Patrizia  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Fawn

**Animal ID:** 35137733  
**Sample Location:** Side  
**Sample Date:** 04/28/18  
**Age:** 05/25/16

### Laboratory Data

<b>Mean Fiber Diameter:</b>	17.1 microns	<b>Fibers Greater Than 30 microns:</b>	0.4 %
<b>Standard Deviation:</b>	3.5 microns	<b>Comfort Factor:</b>	99.6 %
<b>Coefficient of Variation:</b>	20.3 %	<b>Mean Curvature:</b>	48.0 deg/mm
<b>Spin Fineness:</b>	16.5 microns	<b>SD Curvature:</b>	24.2 deg/mm

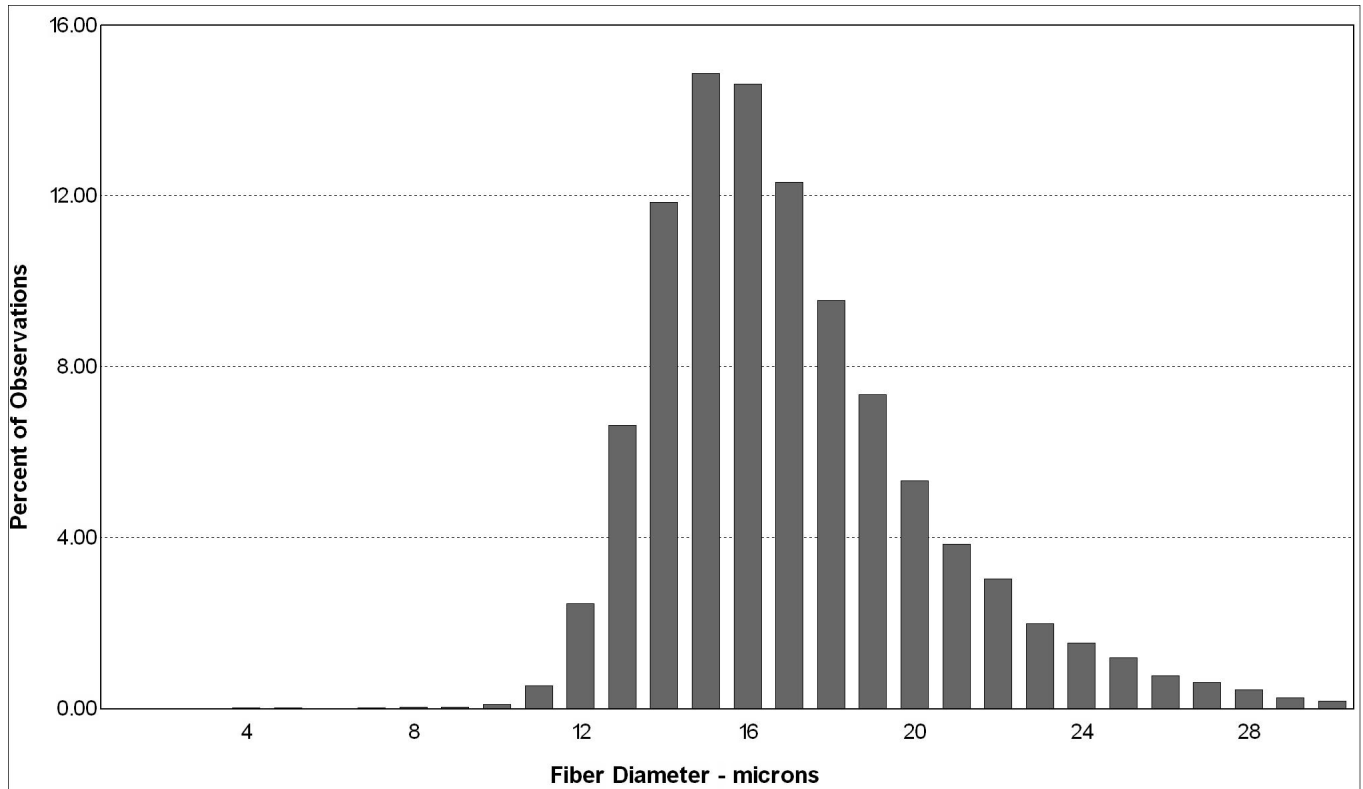

This Test Performed According to I.W.T.O Method 47