

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Glengary Farm Alpacas/Patrick Cassese
2704 Slessman Drive
Plymouth OH 44865 USA

06/25/13

Test No: 458849


Animal and Sample Description

Animal Name: GGF Accoyo Stratosphere's Massimo
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Fawn

Animal ID: 1350203
Sample Location: Side
Sample Date: 04/27/13
Age: 10/14/11

Laboratory Data

Mean Fiber Diameter: 19.3 microns
Standard Deviation: 3.3 microns
Coefficient of Variation: 17.3 %
Fibers Greater Than 30 microns: 0.9 %

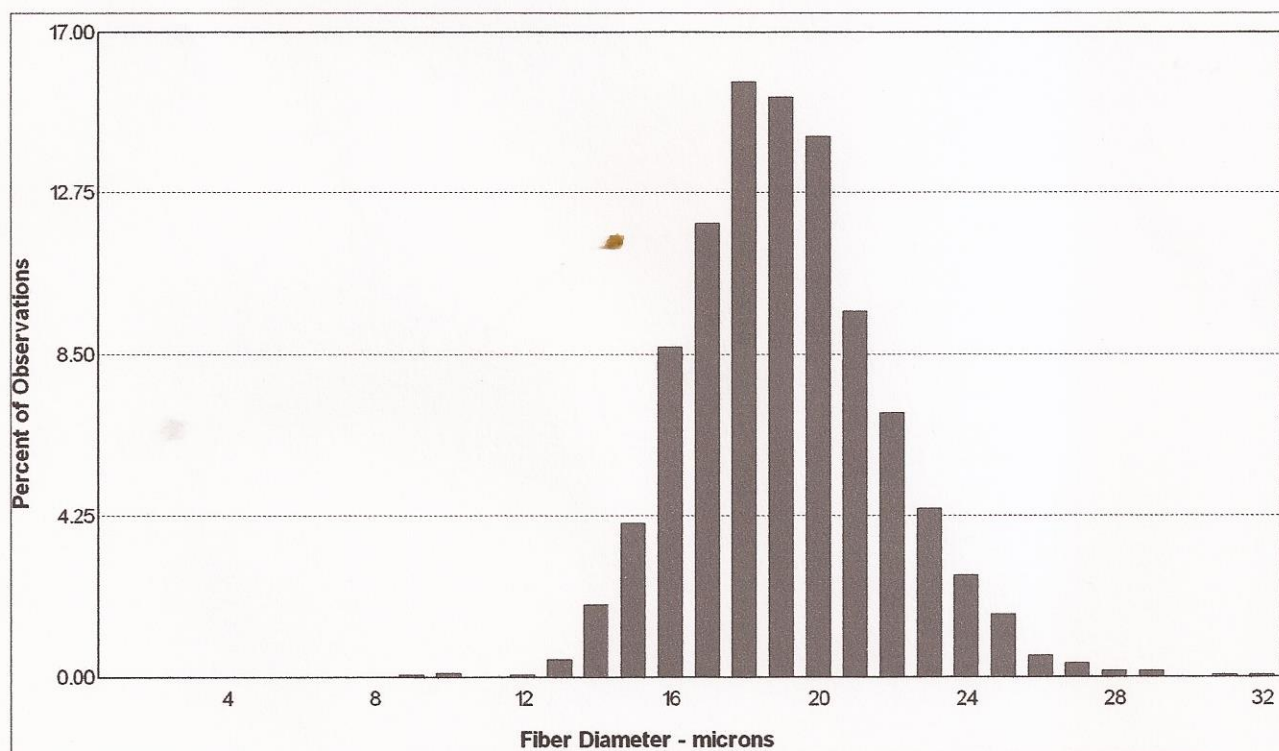

This Test Performed According to I.W.T.O Method 12