



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Glengary Farm Alpacas/Patrick Cassese
2704 Slessman Drive
Plymouth OH 44865 USA

Date: 07/03/18

Test No: 962512


Animal and Sample Description

Animal Name: GGF Fusion by Quixotic
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Grey

Animal ID: 35453793
Sample Location: Side
Sample Date: 04/28/18
Age: 06/26/17

Laboratory Data

Mean Fiber Diameter:	20.7 microns	Fibers Greater Than 30 microns:	4.5 %
Standard Deviation:	4.9 microns	Comfort Factor:	95.5 %
Coefficient of Variation:	23.4 %	Mean Curvature:	37.5 deg/mm
Spin Fineness:	20.6 microns	SD Curvature:	23.1 deg/mm

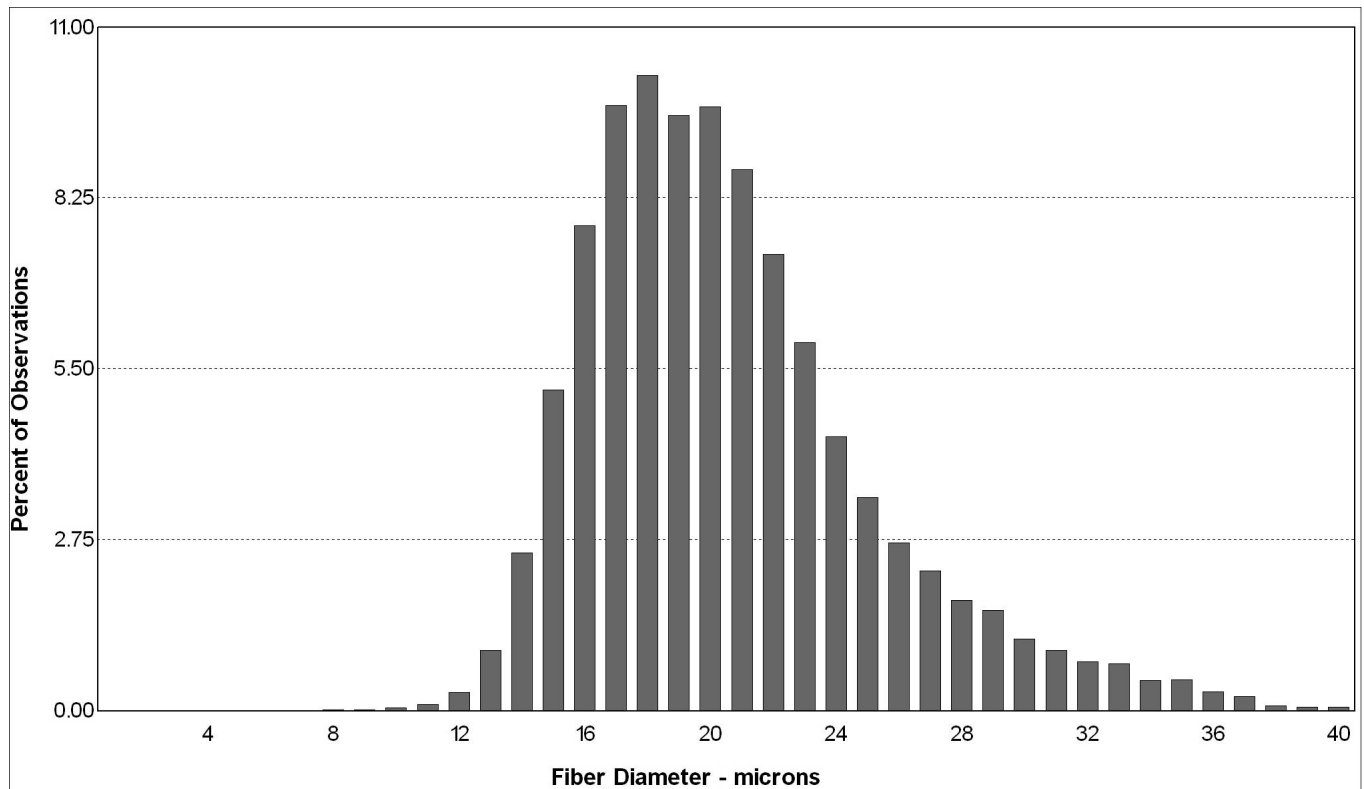

This Test Performed According to I.W.T.O Method 47