



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Glengary Farm Alpacas/Patrick Cassese
2704 Slessman Drive
Plymouth OH 44865 USA

Date: 07/03/18

Test No: 962516


Animal and Sample Description

Animal Name: GGF Primo's Renata
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 35094029
Sample Location: Side
Sample Date: 04/28/18
Age: 09/06/16

Laboratory Data

Mean Fiber Diameter:	20.0 microns	Fibers Greater Than 30 microns:	2.1 %
Standard Deviation:	4.4 microns	Comfort Factor:	97.9 %
Coefficient of Variation:	21.7 %	Mean Curvature:	39.9 deg/mm
Spin Fineness:	19.6 microns	SD Curvature:	21.8 deg/mm

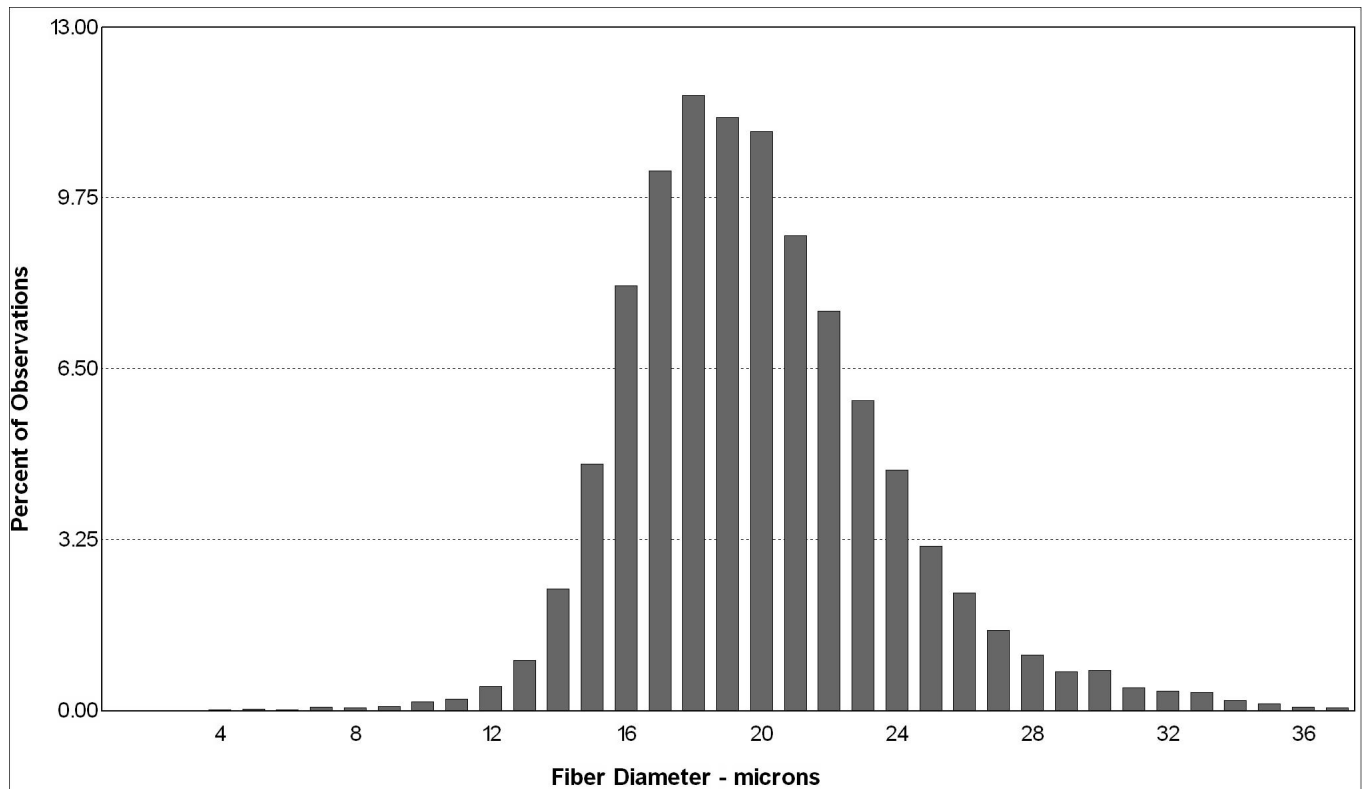

This Test Performed According to I.W.T.O Method 47