

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Glengary Farm Alpacas/Patrick Cassese
2704 Slessman Drive
Plymouth OH 44865 USA

Date: 07/03/18

Test No: 962518


Animal and Sample Description

Animal Name: GGF Midnight Express by Blackbeard
Breed: Alpaca(Huacaya)
Sex: Male
Color: Black

Animal ID: 35453857
Sample Location: Side
Sample Date: 04/28/18
Age: 04/29/17

Laboratory Data

Mean Fiber Diameter:	20.3 microns	Fibers Greater Than 30 microns:	0.8 %
Standard Deviation:	3.1 microns	Comfort Factor:	99.2 %
Coefficient of Variation:	15.4 %	Mean Curvature:	32.5 deg/mm
Spin Fineness:	18.9 microns	SD Curvature:	20.7 deg/mm

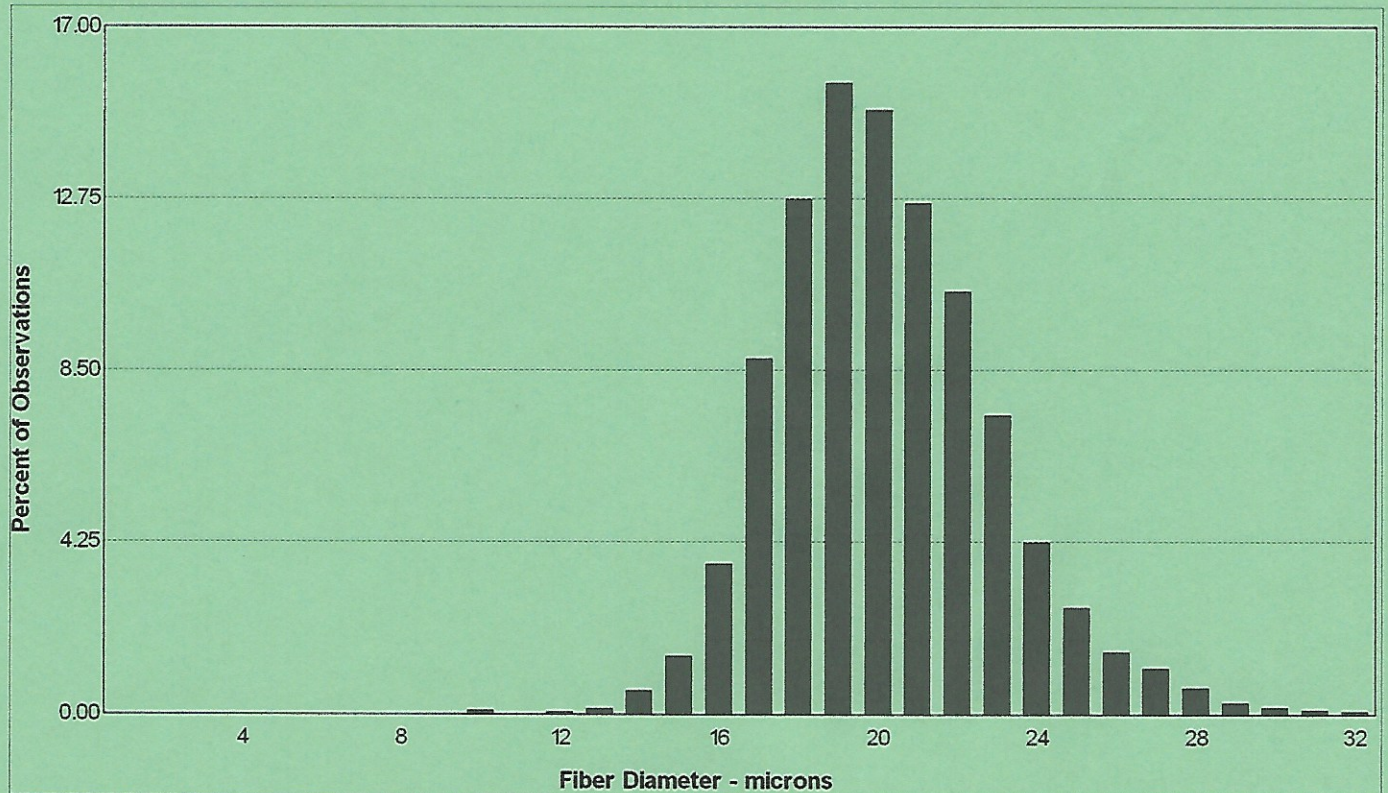

This Test Performed According to I.W.T.O Method 47