



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Woody Acres/David Wood
Box 12, RR5 LCD Main
Saskatoon SK S7K 3J8 Canada

Date: 08/31/17

Test No: 951499


Animal and Sample Description

Animal Name: Dusk (134446450A)
Breed: Alpaca(Huacaya)
Sex: Female
Color: Silver Grey

Animal ID: CAN27460
Sample Location: Mid Side
Sample Date: 06/06/17
Age: 05/19/03

Laboratory Data

Mean Fiber Diameter:	24.5 microns	Fibers Greater Than 30 microns:	7.2 %
Standard Deviation:	4.5 microns	Comfort Factor:	92.8 %
Coefficient of Variation:	18.3 %	Mean Curvature:	39.2 deg/mm
Spin Fineness:	23.3 microns	SD Curvature:	23.5 deg/mm

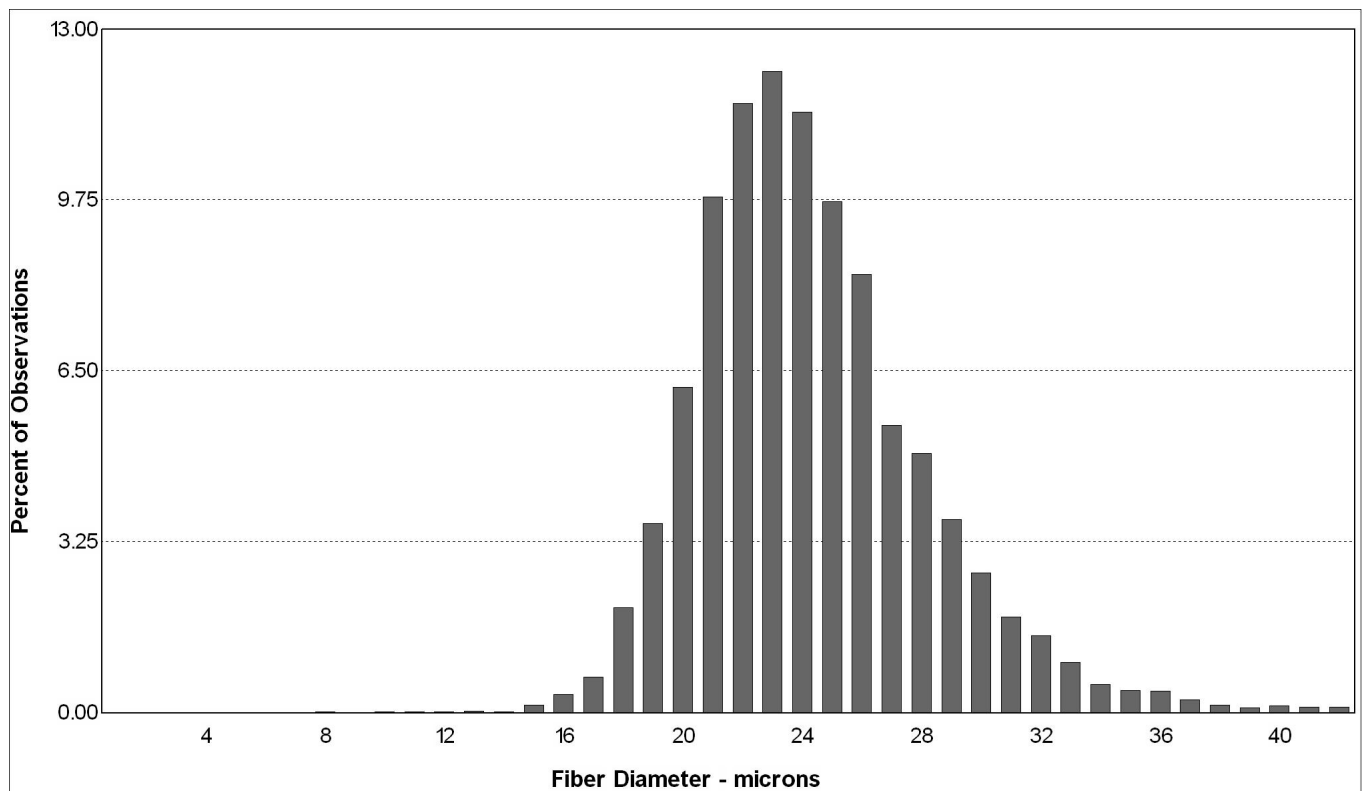

This Test Performed According to I.W.T.O Method 47