



## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

Woody Acres/David Wood  
Box 12, RR5, Stn Main  
Saskatoon SK S7K 3J8 Canada

08/27/08

Test No: 335329


#### Animal and Sample Description

**Animal Name:** Floresa 135679654A  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Dark Brown

**Animal ID:** 30701694  
**Sample Location:** Side (R)  
**Sample Date:** 05/18/08  
**Age:** 08/06/06

#### Laboratory Data

**Mean Fiber Diameter:** 22.7 microns  
**Standard Deviation:** 4.5 microns  
**Coefficient of Variation:** 19.8 %  
**Fibers Greater Than 30 microns:** 6.2 %

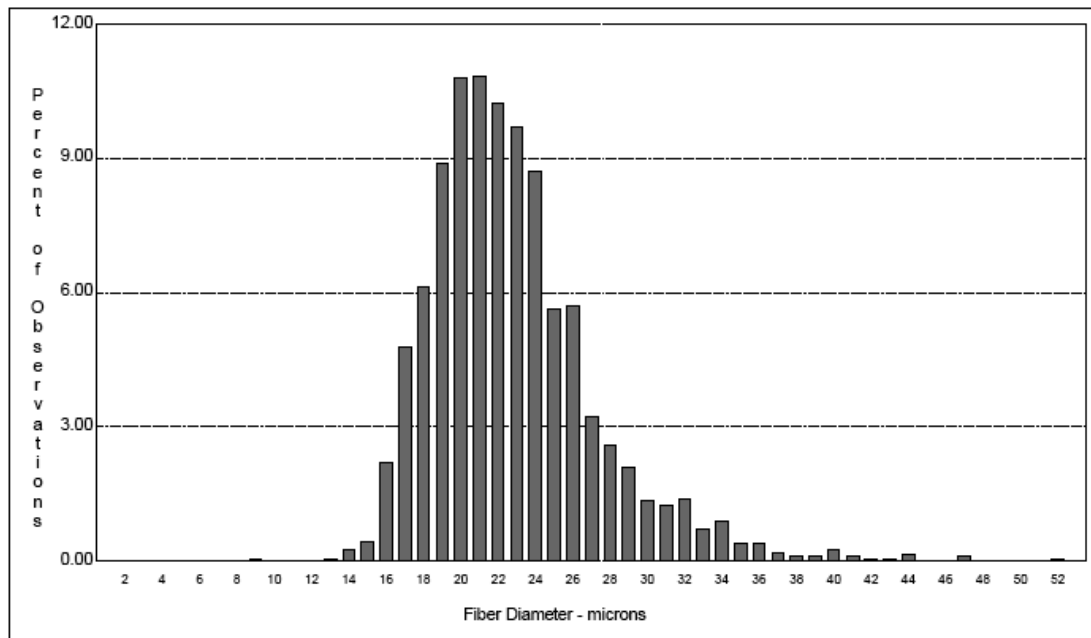

This Test Performed According to I.W.T.O Method 12