



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Woody Acres/David Wood  
Box 12, RR5 LCD Main  
Saskatoon SK S7K 3J8 Canada

**Date:** 08/31/17

**Test No:** 951500


### Animal and Sample Description

**Animal Name:** Grace (135859362A)  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Black

**Animal ID:** CAN29097  
**Sample Location:** Mid Side  
**Sample Date:** 06/03/17  
**Age:** 05/15/04

### Laboratory Data

<b>Mean Fiber Diameter:</b>	28.8 microns	<b>Fibers Greater Than 30 microns:</b>	33.1 %
<b>Standard Deviation:</b>	4.6 microns	<b>Comfort Factor:</b>	66.9 %
<b>Coefficient of Variation:</b>	16.1 %	<b>Mean Curvature:</b>	26.0 deg/mm
<b>Spin Fineness:</b>	27.0 microns	<b>SD Curvature:</b>	16.4 deg/mm

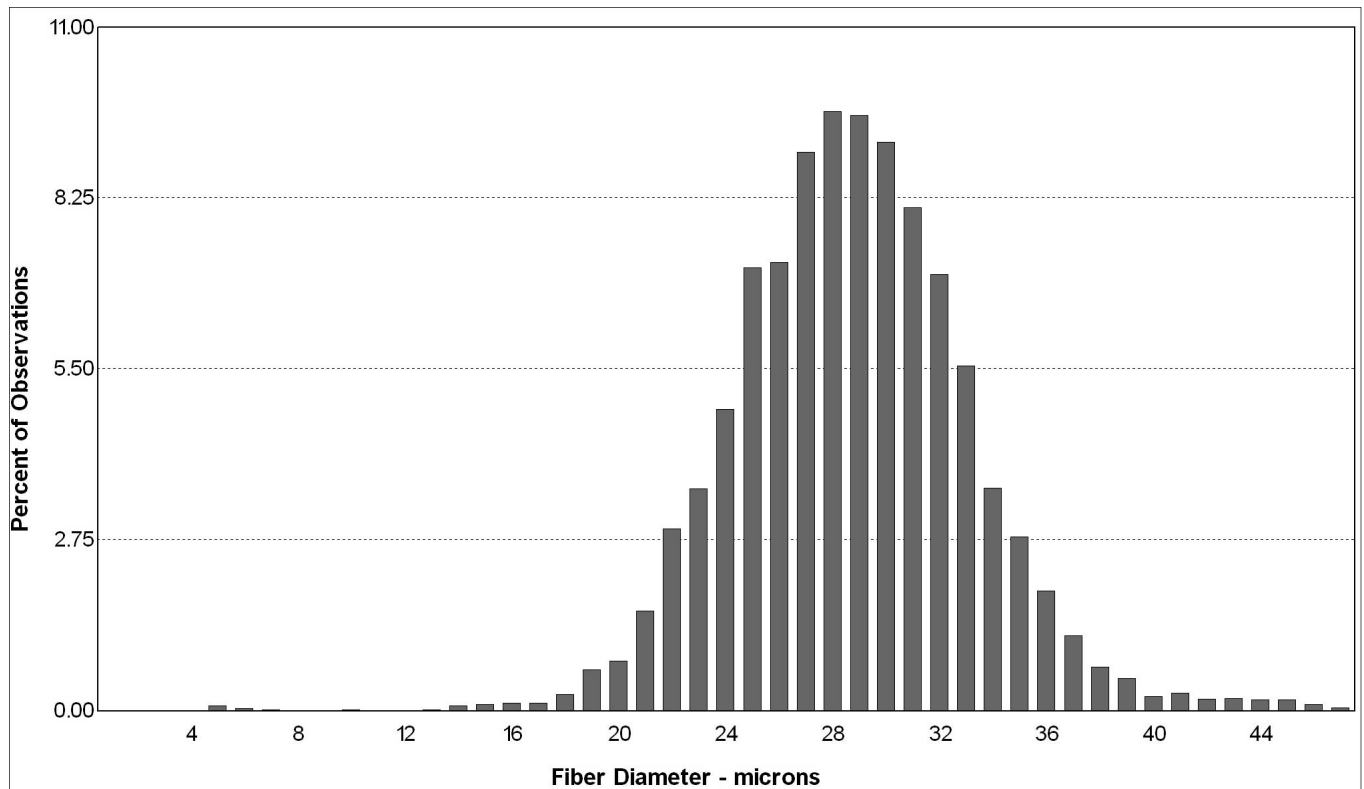

This Test Performed According to I.W.T.O Method 47