



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Woody Acres/David Wood
Box 12, RR5 LCD Main
Saskatoon SK S7K 3J8 Canada

Date: 08/31/17

Test No: 951498


Animal and Sample Description

Animal Name: Patches
Breed: Alpaca(Huacaya)
Sex: Male
Color: Multi

Animal ID: 151601577A
Sample Location: Mid Side
Sample Date: 06/04/17
Age: 07/19/12

Laboratory Data

Mean Fiber Diameter:	26.4 microns	Fibers Greater Than 30 microns:	18.3 %
Standard Deviation:	4.9 microns	Comfort Factor:	81.7 %
Coefficient of Variation:	18.5 %	Mean Curvature:	37.8 deg/mm
Spin Fineness:	25.1 microns	SD Curvature:	23.0 deg/mm

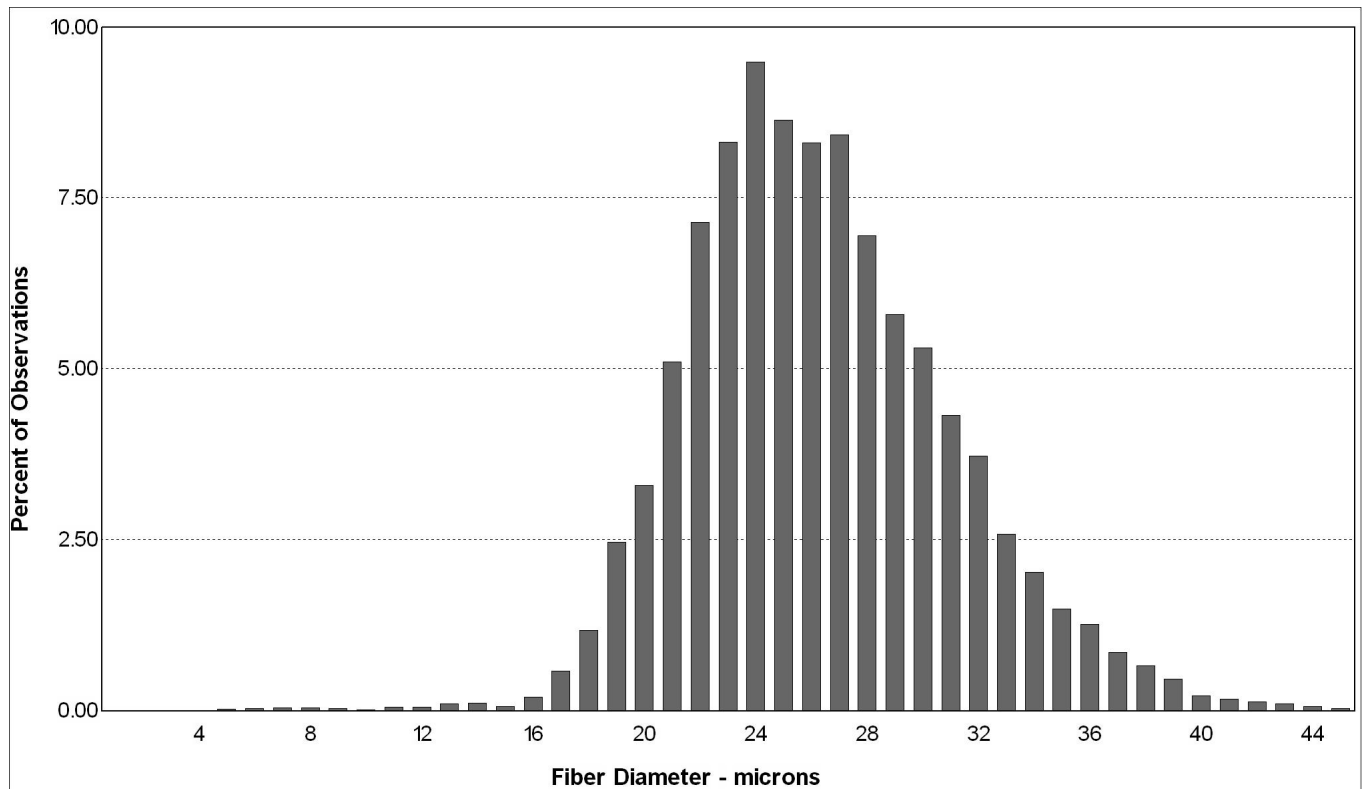

This Test Performed According to I.W.T.O Method 47