



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Woody Acres/David Wood
Box 12, RR5, Stn Main
Saskatoon SK S7K 3J8 Canada

08/27/08

Test No: 335309


Animal and Sample Description

Animal Name: Tammy 131939527A
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 841491
Sample Location: Side (R)
Sample Date: 05/18/08
Age: 08/21/02

Laboratory Data

Mean Fiber Diameter: 27.9 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 16.1 %
Fibers Greater Than 30 microns: 22.7 %

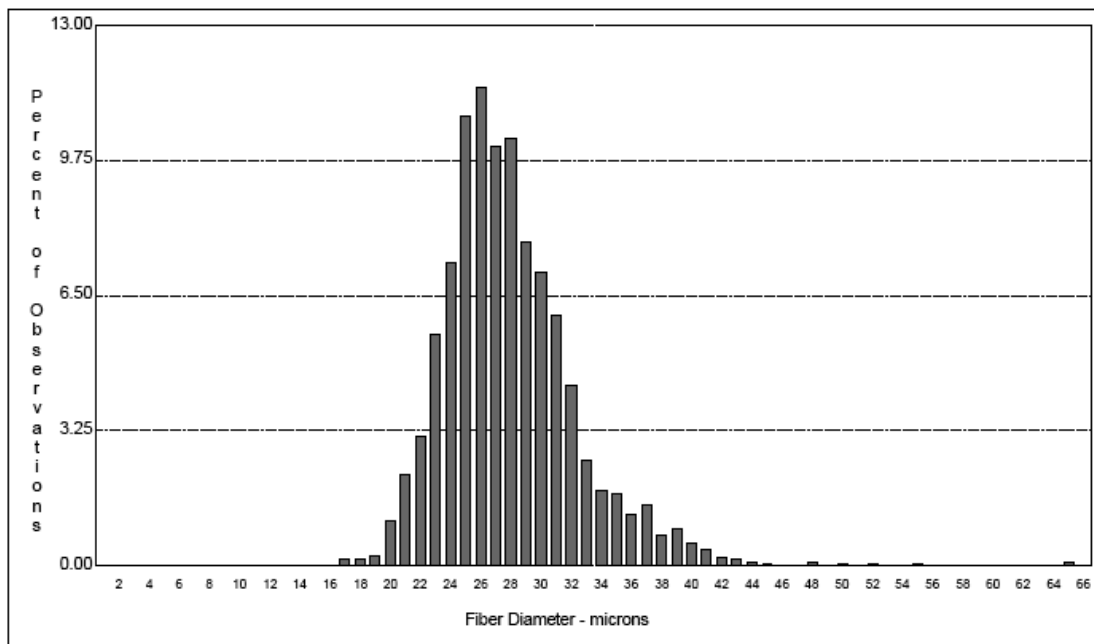

This Test Performed According to I.W.T.O Method 12