



## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

Woody Acres/David Wood  
Box 12, RR5, Stn Main  
Saskatoon SK S7K 3J8 Canada

08/27/08

Test No: 335310


#### Animal and Sample Description

**Animal Name:** Tanya 131939617A  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** White

**Animal ID:** 841492  
**Sample Location:** Side (R)  
**Sample Date:** 05/17/08  
**Age:** 07/23/02

#### Laboratory Data

**Mean Fiber Diameter:** 27.9 microns  
**Standard Deviation:** 4.4 microns  
**Coefficient of Variation:** 15.8 %  
**Fibers Greater Than 30 microns:** 23.9 %

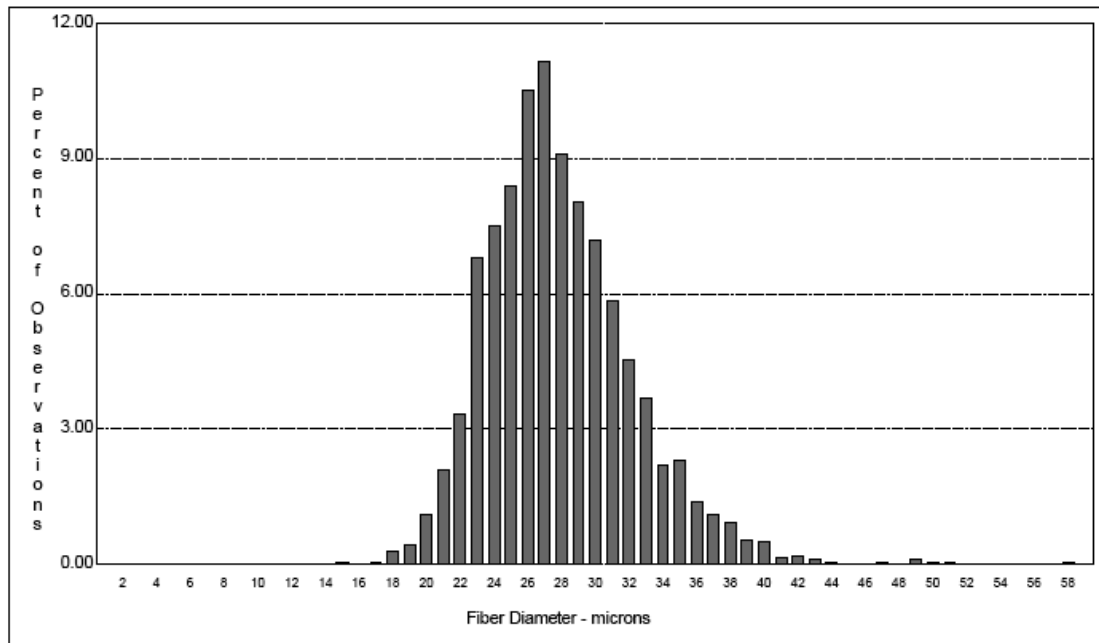

This Test Performed According to I.W.T.O Method 12