



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Woody Acres/David Wood
Box 12, RR5, Stn Main
Saskatoon SK S7K 3J8 Canada

08/27/08

Test No: 335326


Animal and Sample Description

Animal Name: Tarracotta 135679112A
Breed: Alpaca(Huacaya)
Sex: Male
Color: Dark Fawn

Animal ID: 30701625
Sample Location: Side (R)
Sample Date: 05/13/08
Age: 06/29/06

Laboratory Data

Mean Fiber Diameter: 25.8 microns
Standard Deviation: 4.9 microns
Coefficient of Variation: 19.0 %
Fibers Greater Than 30 microns: 13.3 %

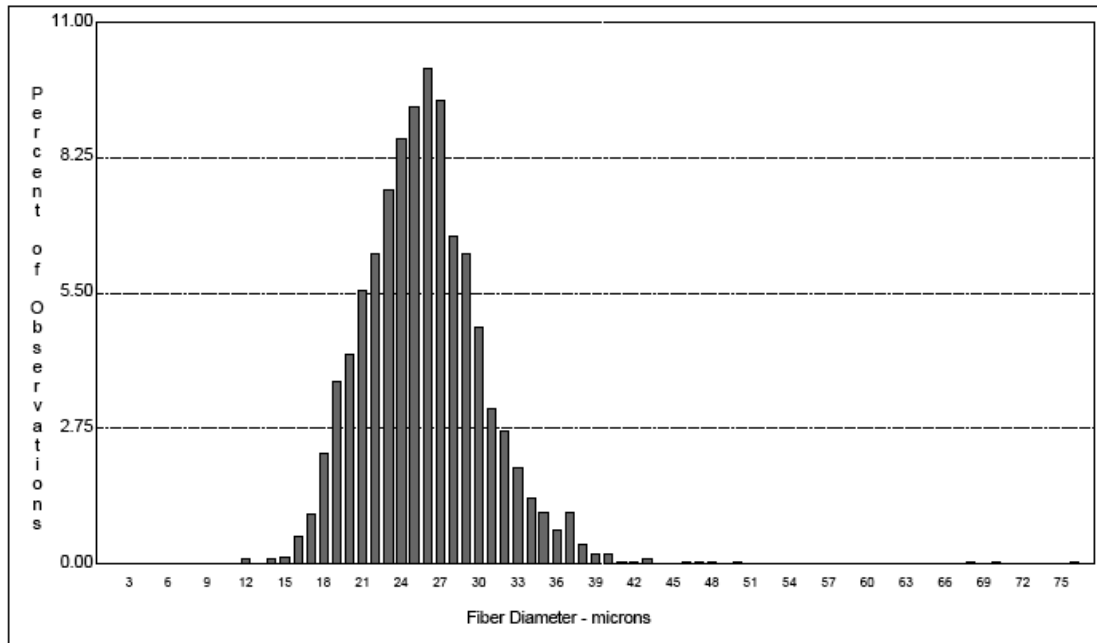

This Test Performed According to I.W.T.O Method 12