



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Delphi Alpacas/Linda Bat
P.O. Box 9
Coaldale CO 81222

11/17/08

Test No: 341708

Animal and Sample Description


Animal Name: Cheyenne
Breed: Alpaca(Huacaya)
Sex: Female
Color: Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 11/13/08
Age: XXXXX

9/6/05 DOB

Laboratory Data

Mean Fiber Diameter: 25.7 microns
Standard Deviation: 4.0 microns
Coefficient of Variation: 15.6 %
Fibers Greater Than 30 microns: 11.3 %

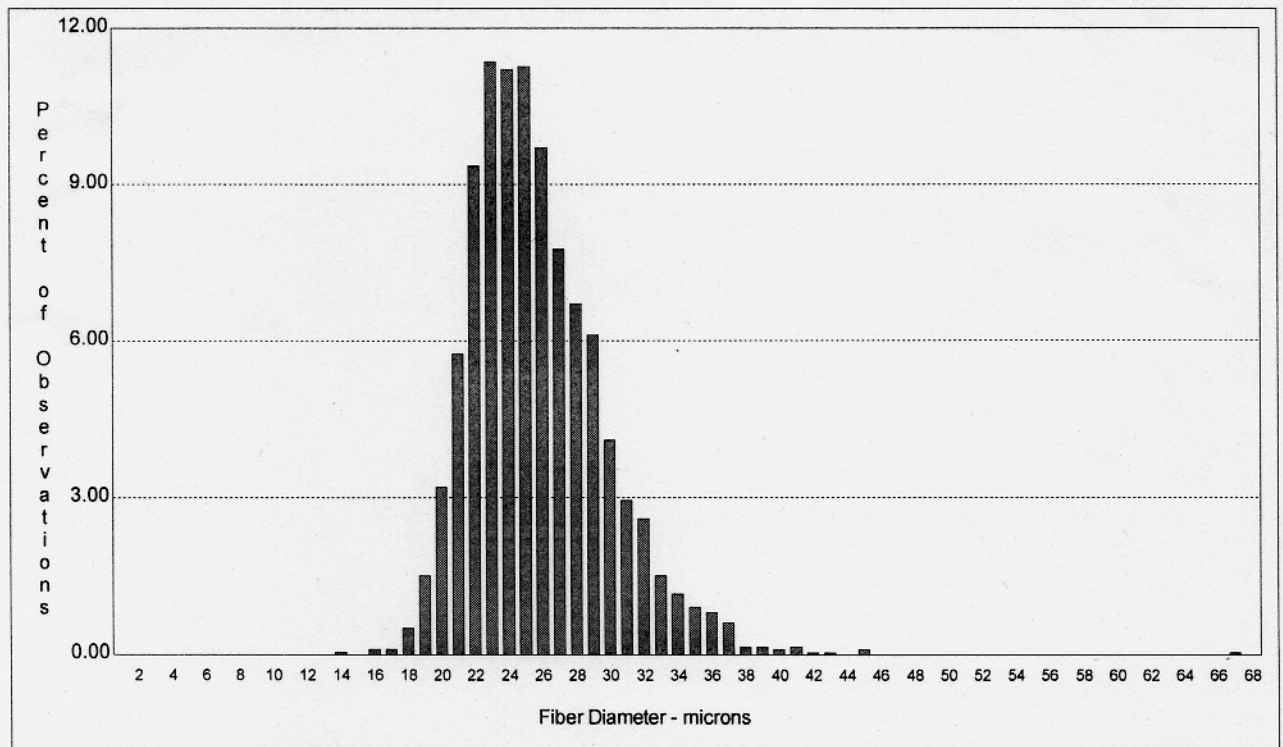

This Test Performed According to I.W.T.O Method 12