



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Mystic Mountain Alpacas/Michael Hall
17227 Hwy 36
Covington GA 30014 USA

04/23/12

Test No: 427560


Animal and Sample Description

Animal Name: Mystic Mountain's Khryton
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: 31930734
Sample Location: Side
Sample Date: 04/10/12
Age: 03/10/11

Laboratory Data

Mean Fiber Diameter: 19.3 microns
Standard Deviation: 4.2 microns
Coefficient of Variation: 21.5 %
Fibers Greater Than 30 microns: 1.1 %

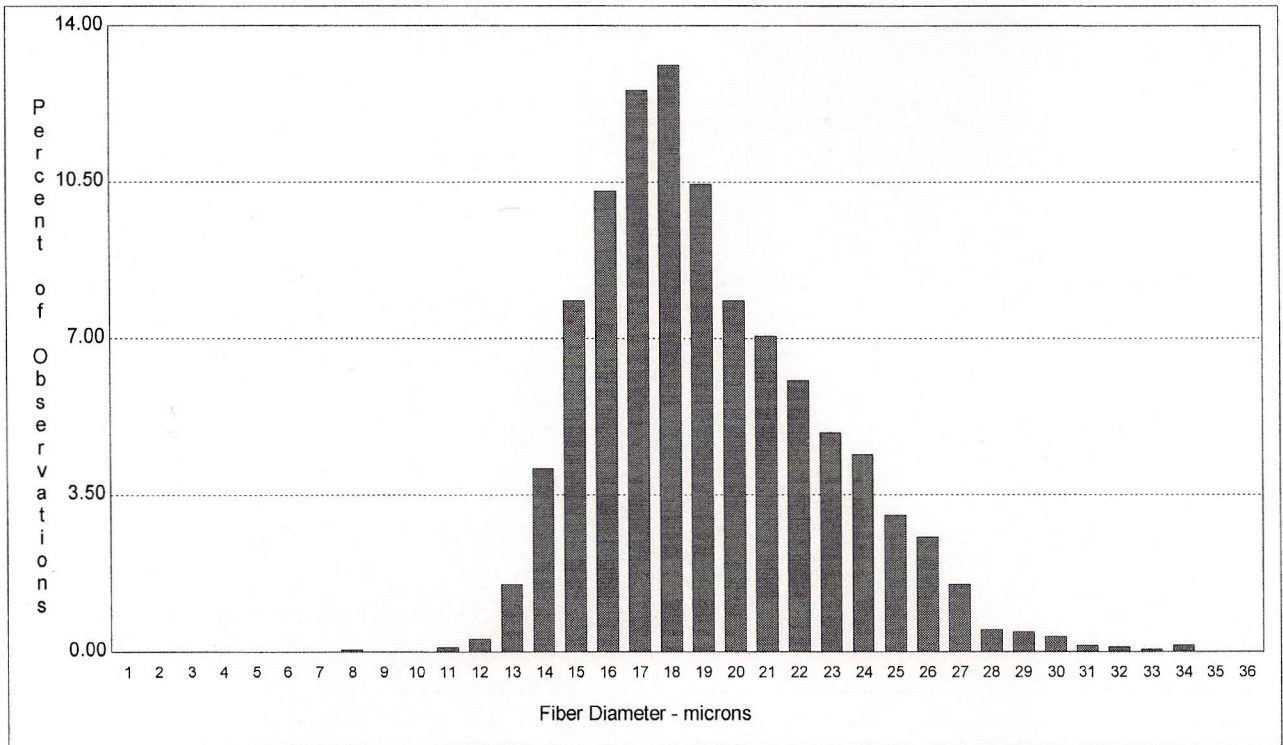

This Test Performed According to I.W.T.O Method 12