



Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

Siroian Laserscan
 Micron Test Report

Querencia/Dennis & Marie Hurley
 33530 Mt Tom Dr
 Harrisburg OR 97446

Test No: 459143


06/28/13

Animal and Sample Description

Animal Name: Abrazo Royale of Querencia
Breed: Alpaca(Huacaya)
Sex: Male
Color: LF
Animal ID: 32121490
Sample Location: Side
Sample Date: 05/28/13
Age: 06/08/11

Laboratory Data

Mean Fiber Diameter: 18.4 microns
Standard Deviation: 3.5 microns
Coefficient of Variation: 18.8 %
Fibers Greater Than 30 microns: 1.0 %

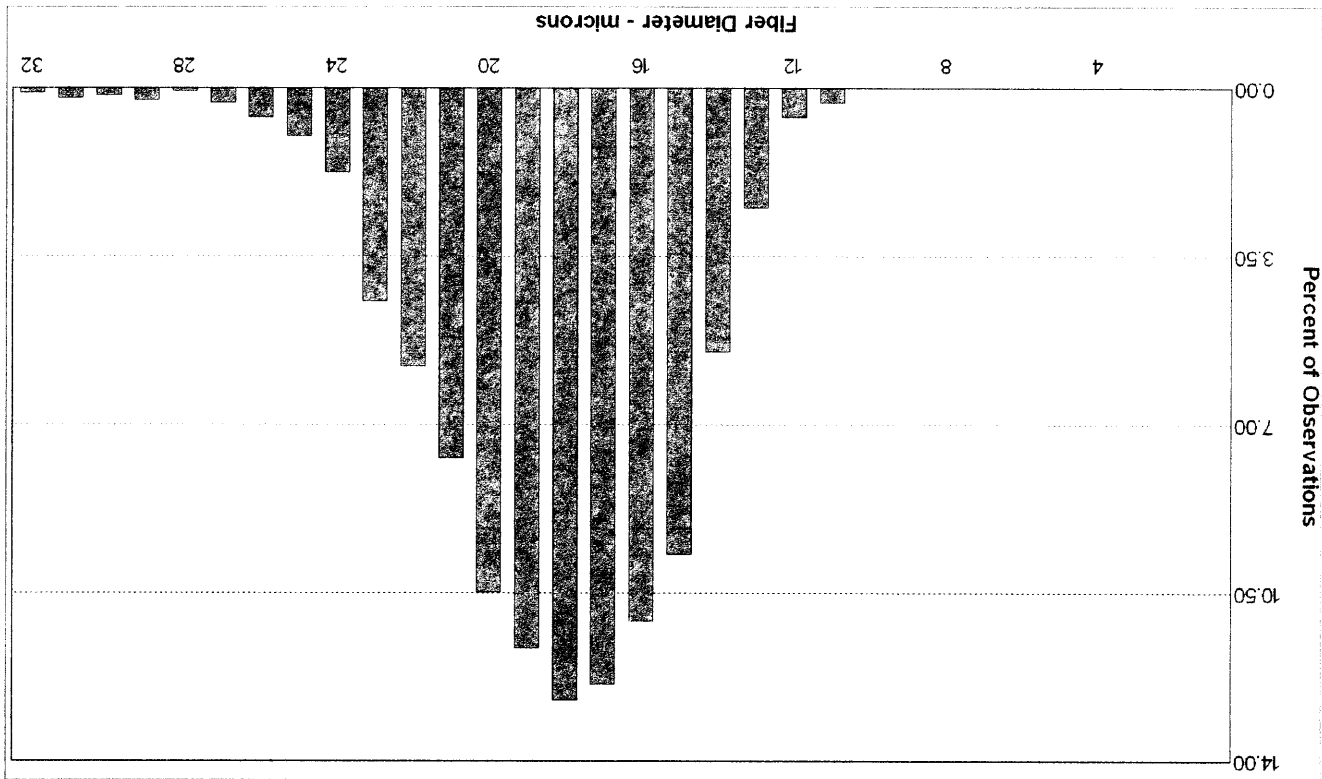

This Test Performed According to I.W.T.O Method 12