

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Heart's Desire Farm, LLC/Mike Harnett
Rt 2, Box 750
Shinnston WV 26431 USA

08/16/10

Test No: 388922


Animal and Sample Description

Animal Name: HDF Accoyo OBI-WAN
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/14/10
Age: 06/03/08

Laboratory Data

Mean Fiber Diameter: 18.8 microns
Standard Deviation: 4.0 microns
Coefficient of Variation: 21.1 %
Fibers Greater Than 30 microns: 1.2 %

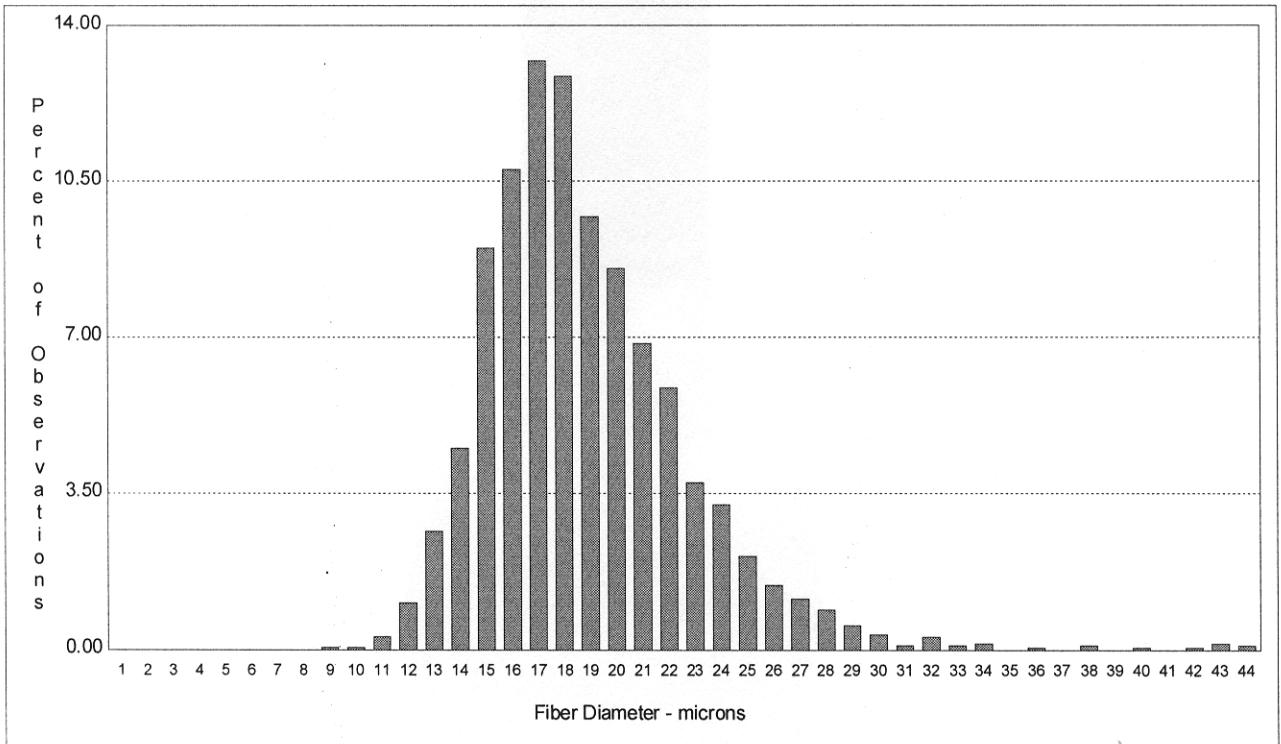

This Test Performed According to I.W.T.O Method 12