

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Hearts Desire Farm Colorado/Deb Dorband
928 S CR 31
Berthoud CO 80513

07/26/11

Test No: 411080


Animal and Sample Description

Animal Name: HDF Florrie
Breed: Alpaca(Huacaya)
Sex: Female
Color: Dark Fawn

Animal ID: 32062328
Sample Location: Side
Sample Date: 04/29/11
Age: 07/17/09

Laboratory Data

Mean Fiber Diameter: 20.1 microns
Standard Deviation: 3.9 microns
Coefficient of Variation: 19.6 %
Fibers Greater Than 30 microns: 1.3 %

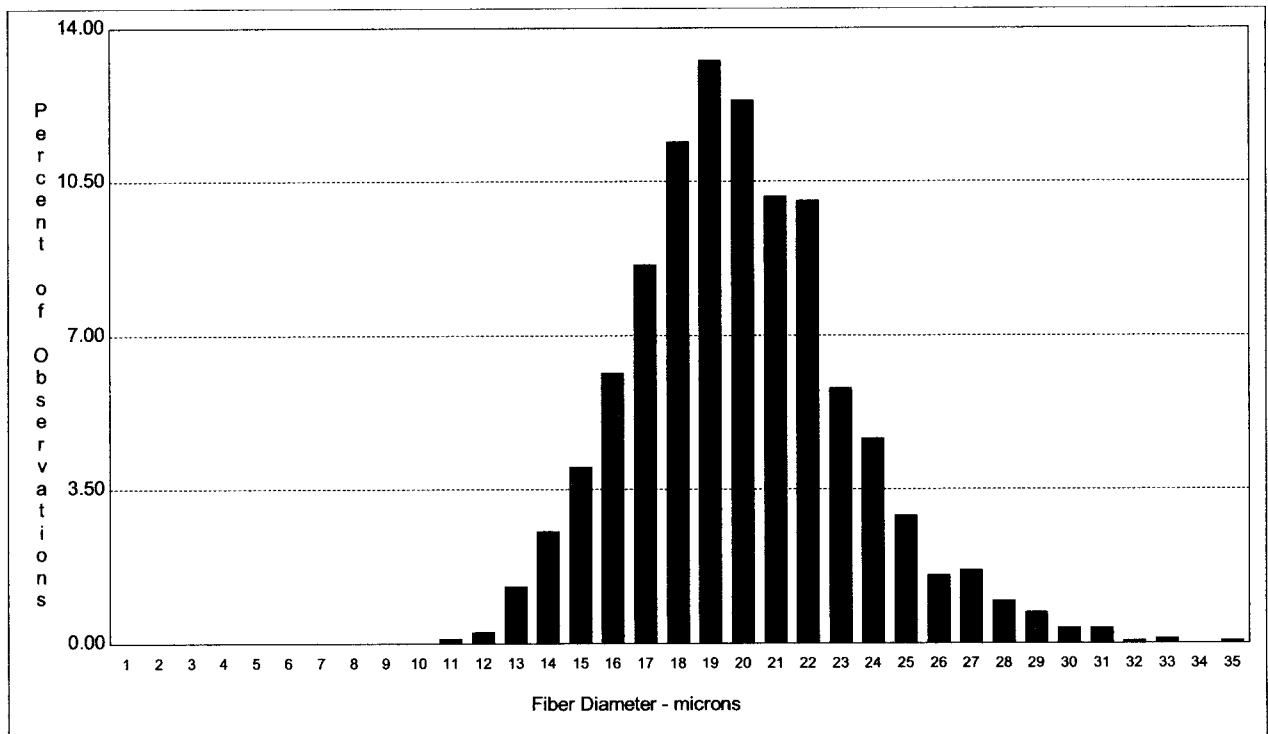

This Test Performed According to I.W.T.O Method 12