



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Pucara International/Jude Anderson & Alan Cousill  
15204 SW Muddy Valley Road  
McMinnville OR 97128-8521

07/30/10

Test No: 386633


### Animal and Sample Description

**Animal Name:** E67 Pucara Beachwood Honolua  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** White

**Animal ID:** 32079562  
**Sample Location:** Side  
**Sample Date:** 06/01/09  
**Age:** 08/01/09

### Laboratory Data

**Mean Fiber Diameter:** 21.2 microns  
**Standard Deviation:** 3.9 microns  
**Coefficient of Variation:** 18.6 %  
**Fibers Greater Than 30 microns:** 3.4 %

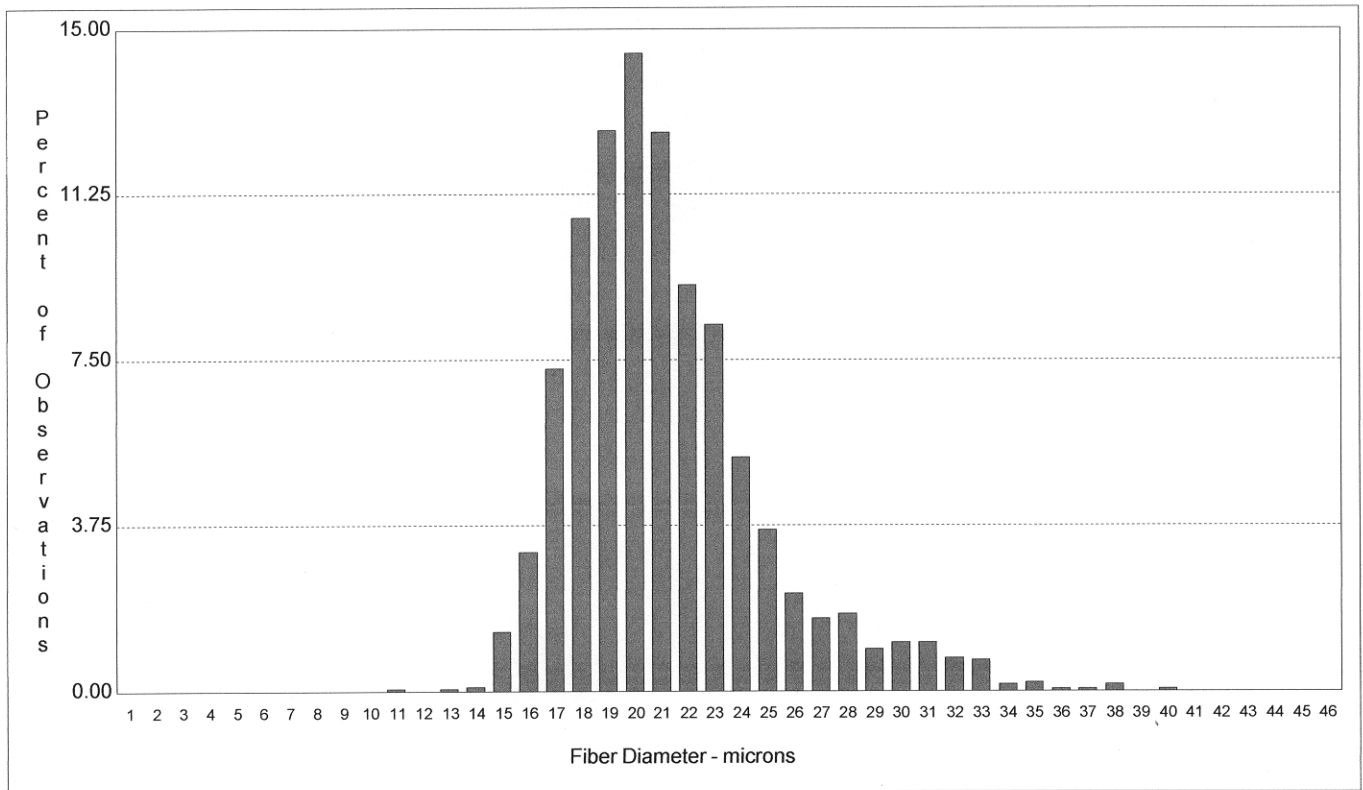

This Test Performed According to I.W.T.O Method 12