

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Mountain Sky Ranch/Deb Dorband
928 S CR 31
Berthoud CO 80513

09/14/10

Test No: 391224


Animal and Sample Description

Animal Name: RNA Cara
Breed: Alpaca(Huacaya)
Sex: Female
Color: Bay Black

Animal ID: 30564183
Sample Location: Side
Sample Date: 06/17/10
Age: 06/22/06

Laboratory Data

Mean Fiber Diameter: 29.0 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 15.4 %
Fibers Greater Than 30 microns: 28.4 %

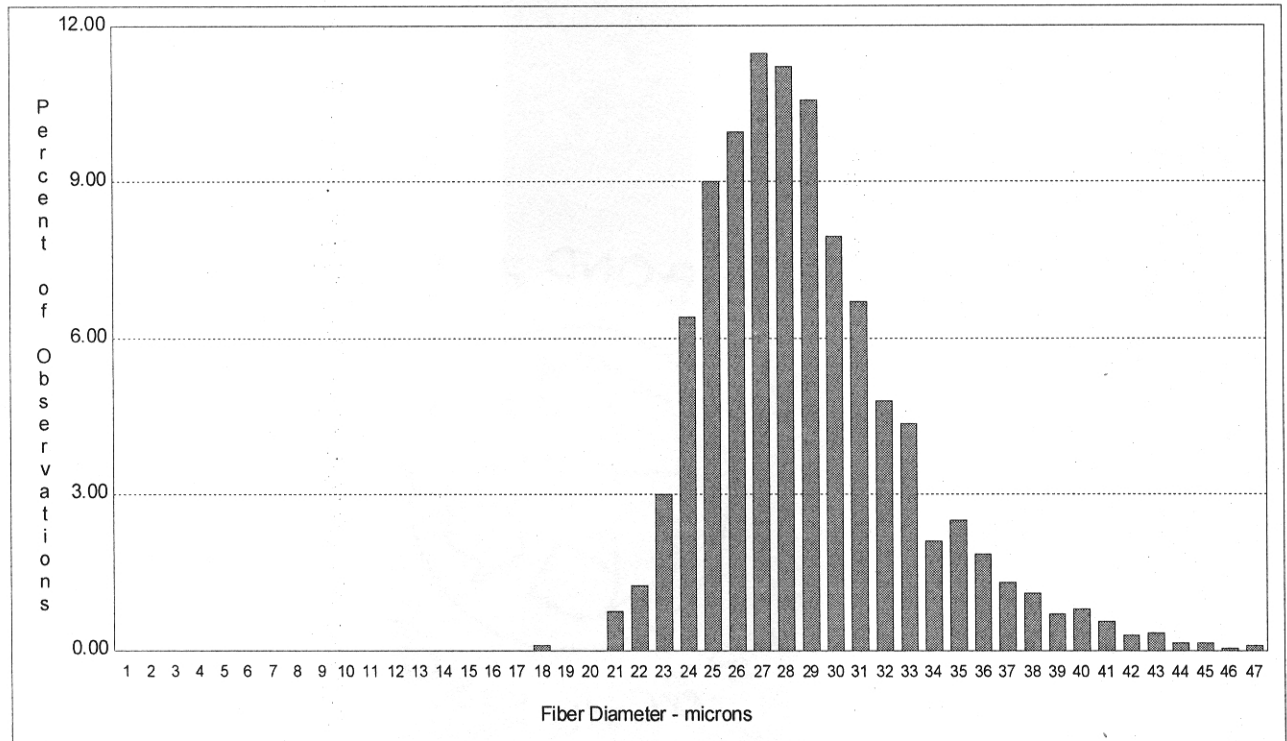

This Test Performed According to I.W.T.O Method 12