

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Mountain Sky Ranch/Deb Dorband
901 S CR 31
Berthoud CO 80513

Date: 11/06/14

Test No: 493345


Animal and Sample Description

Animal Name: PM's Cria (2013)
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: XXXXX
Sample Location: Grid
Sample Date: 05/29/14
Age: 09/22/13

Laboratory Data

Mean Fiber Diameter:	20.7 microns	Fibers Greater Than 30 microns:	5.7 %
Standard Deviation:	5.8 microns	Comfort Factor:	94.3 %
Coefficient of Variation:	28.0 %	Mean Curvature:	37.5 deg/mm
Spin Fineness:	21.5 microns	SD Curvature:	22.3 deg/mm

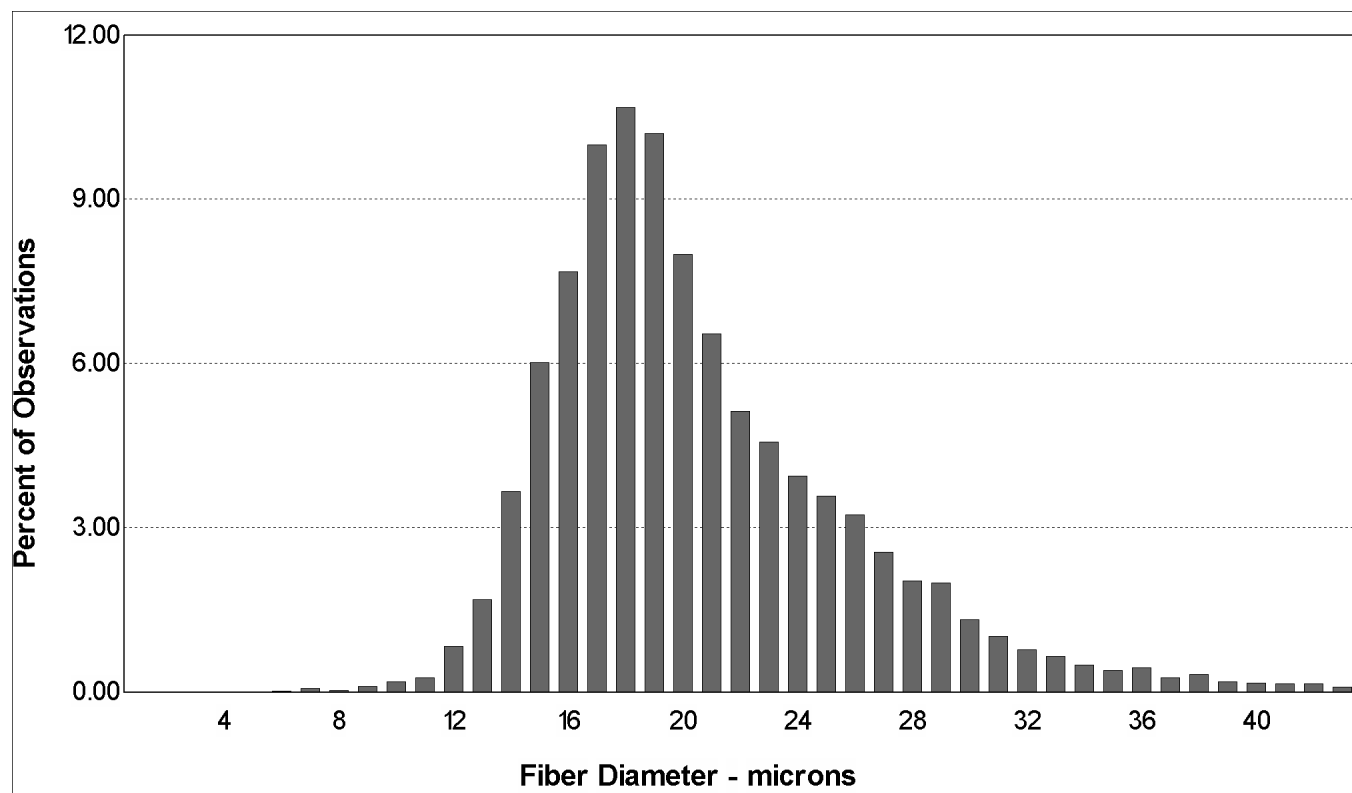

This Test Performed According to I.W.T.O Method 47